

3737
1-40

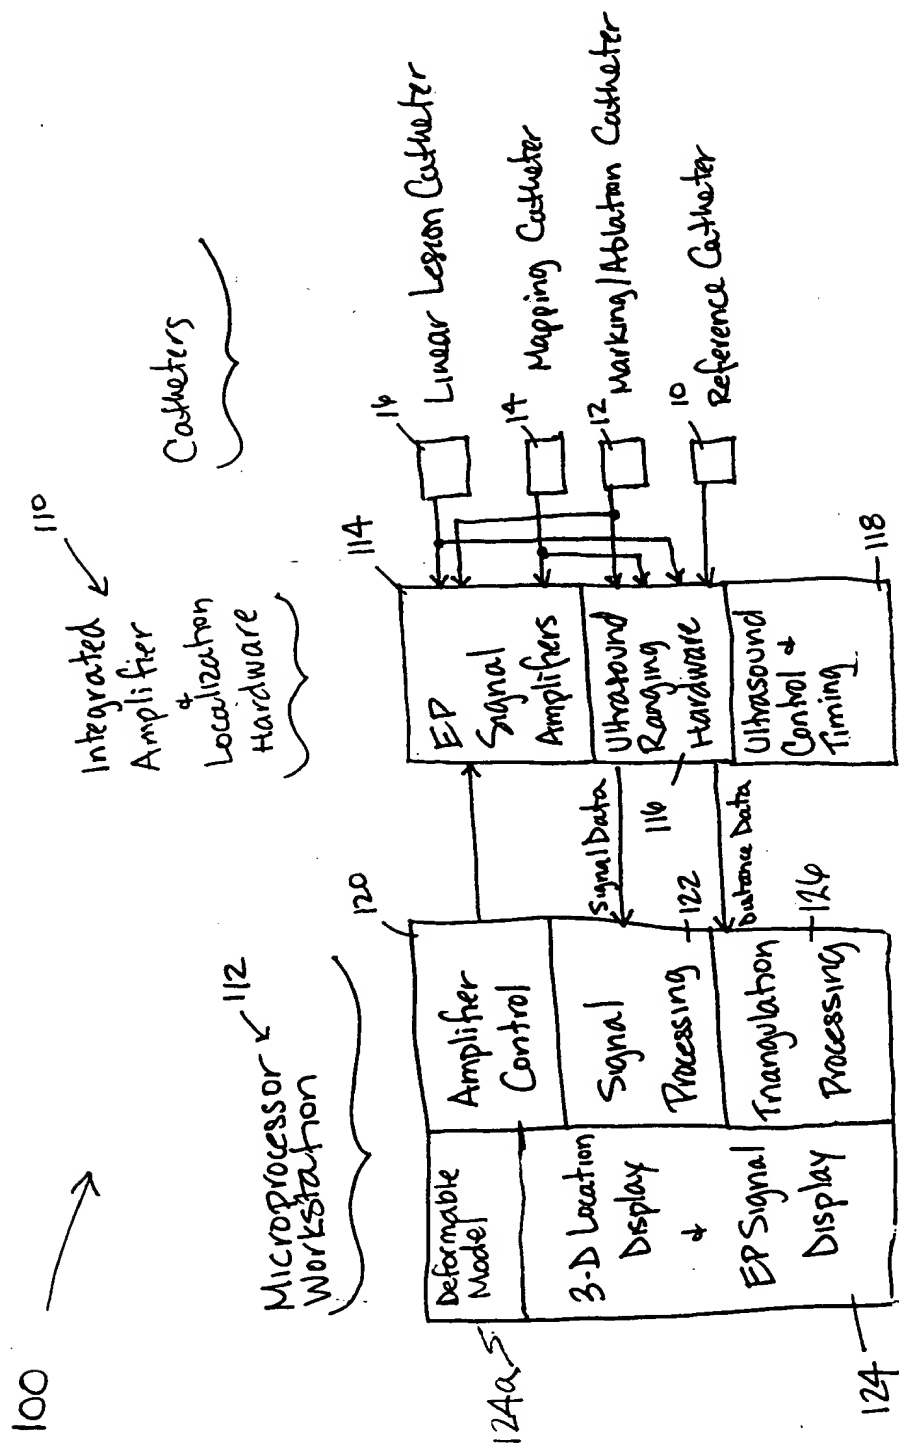


Fig. 1

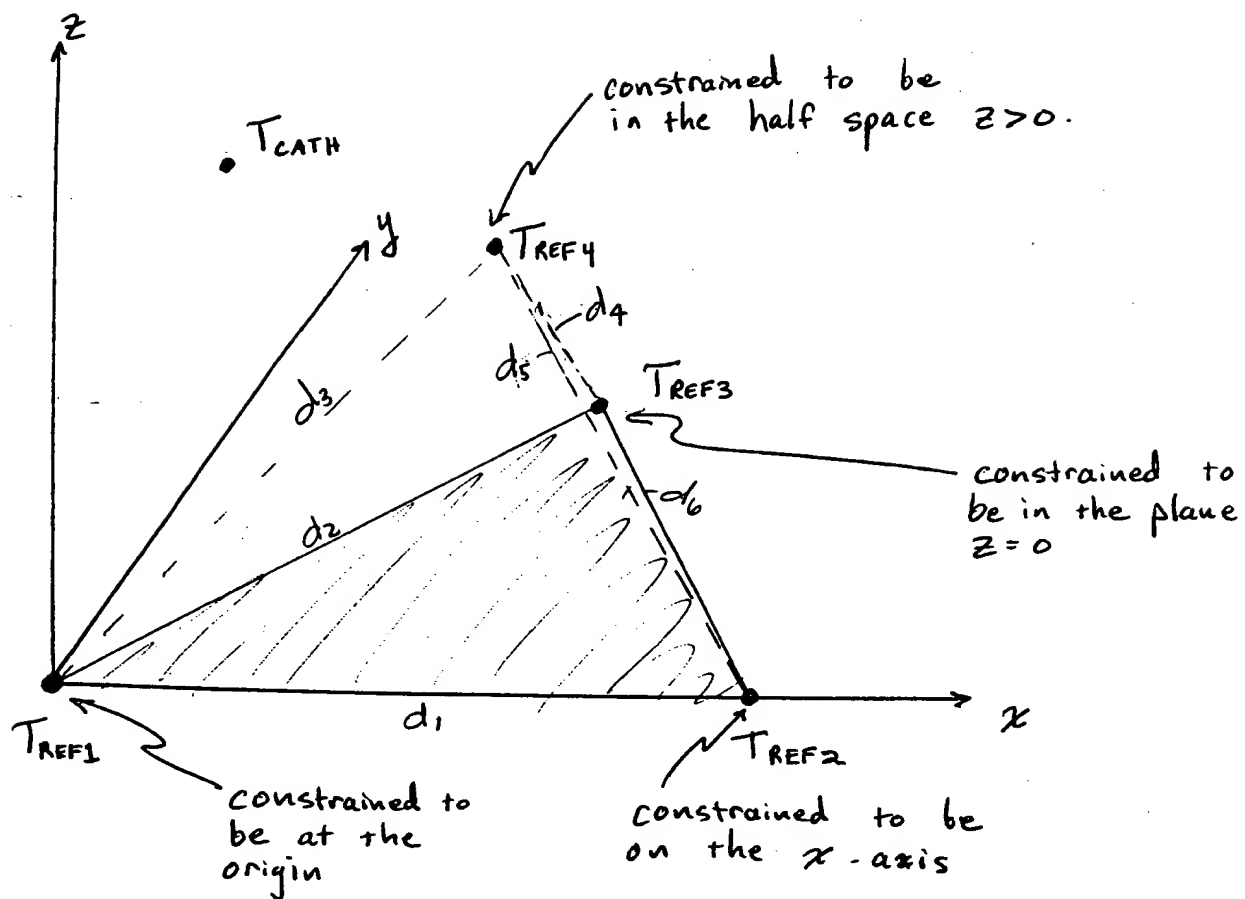


Fig. 2

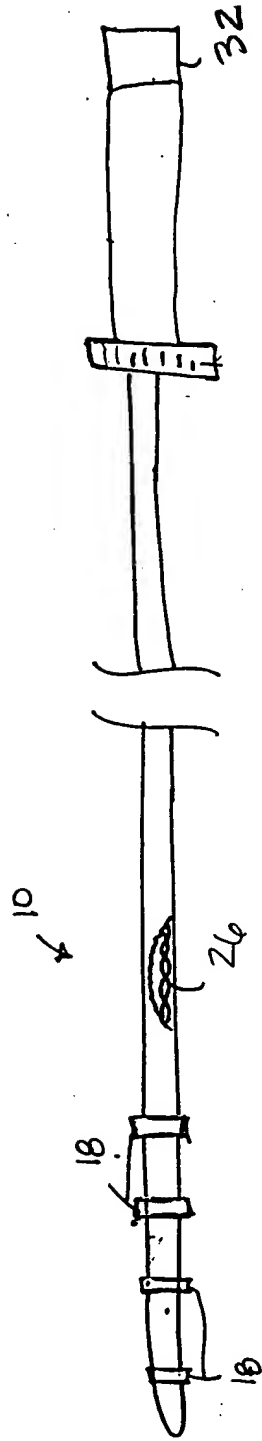


FIG. 3

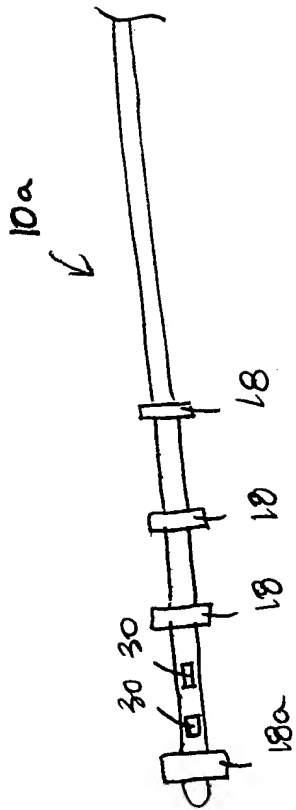


FIG. 4

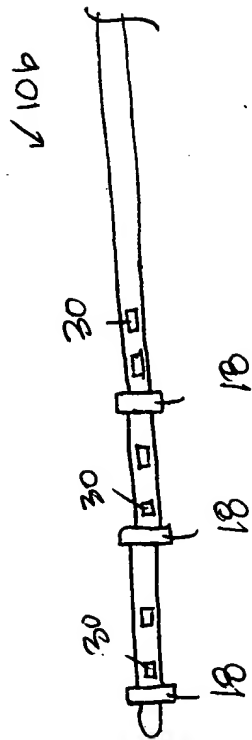


FIG. 5

86E080"40E82T60

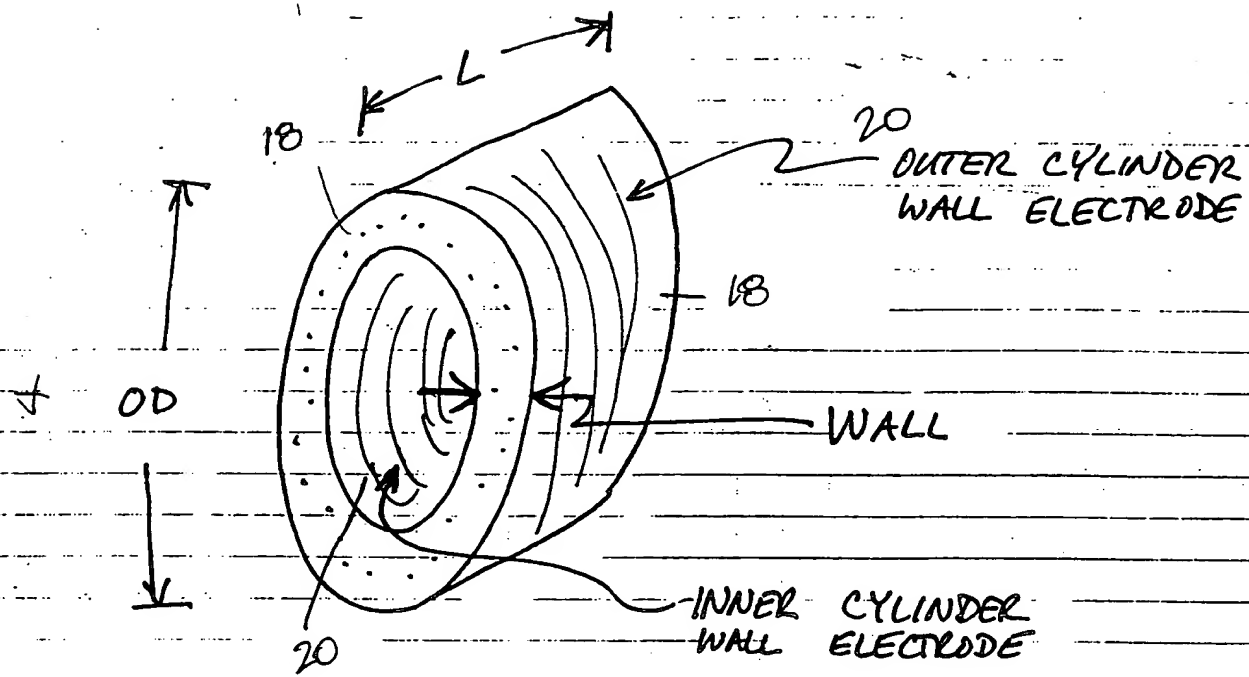


FIGURE 6 PIEZOELECTRIC CYLINDER

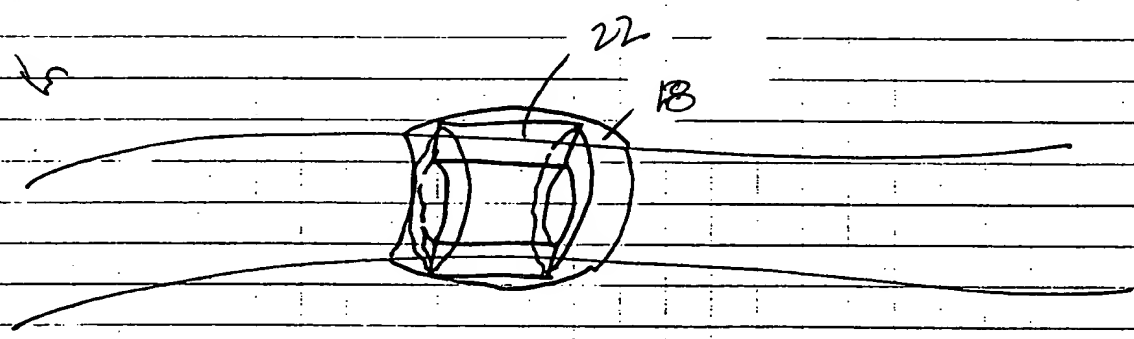


FIGURE 7. TRANSDUCER WITH LENS

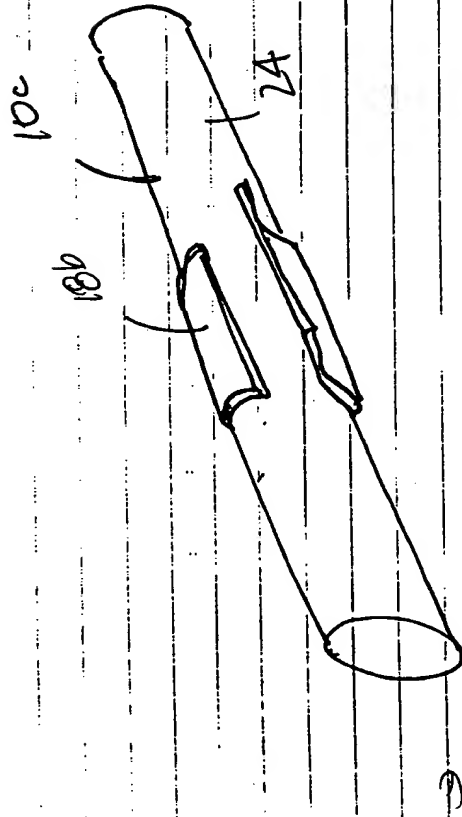


FIGURE 3 POLYMER PIEZOELECTRIC
WRAPPED AROUND
MANDREL

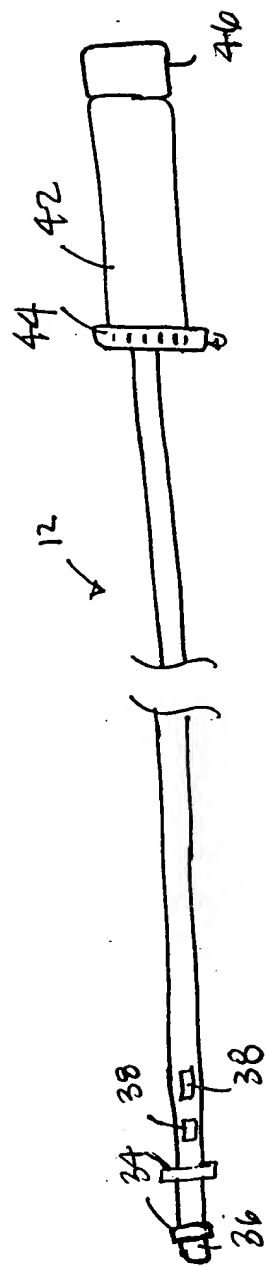


Fig. 9

PIEZOELECTRIC TRANSDUCER 34

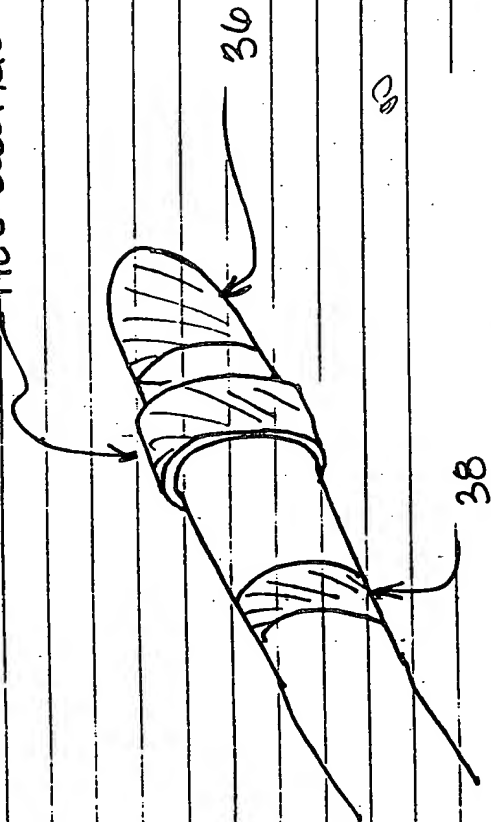


FIGURE 10 DISTAL TRANSDUCER ON

ABLATION CATHETER

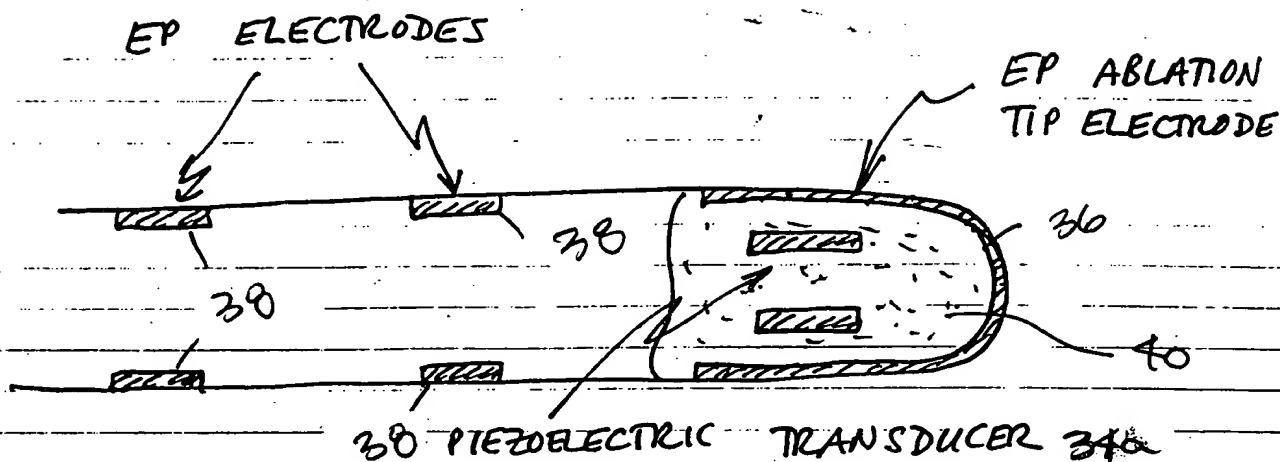


FIGURE 11 DISTAL TRANSDUCER WITH IN ABLATION CATHETER TIP. (CROSS SECTIONAL VIEW)

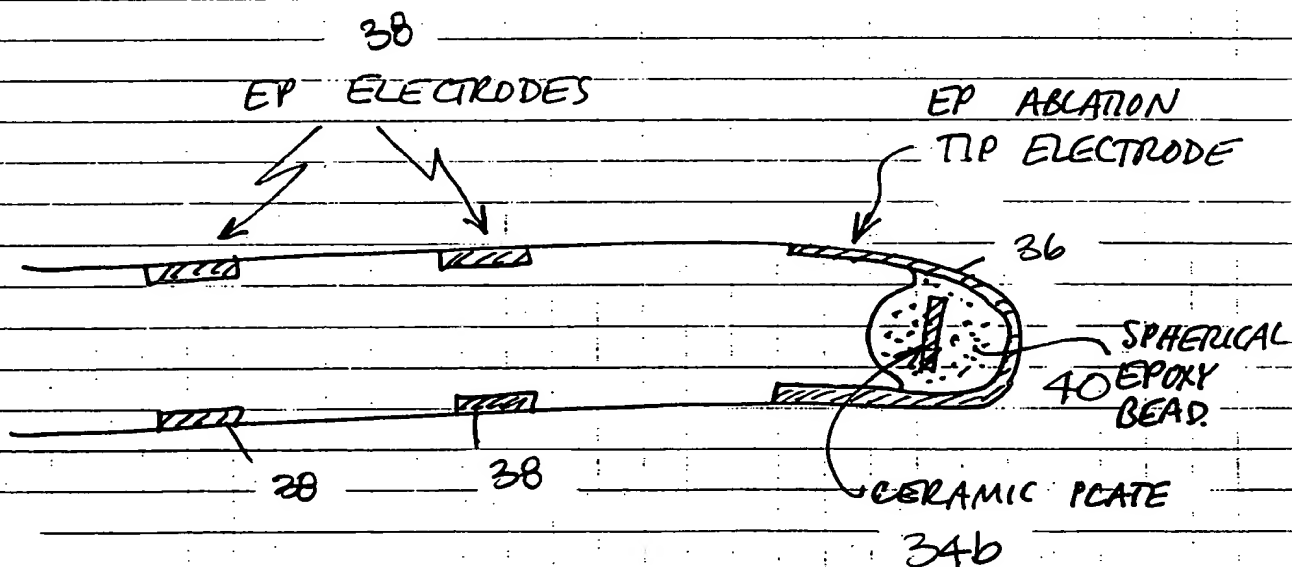
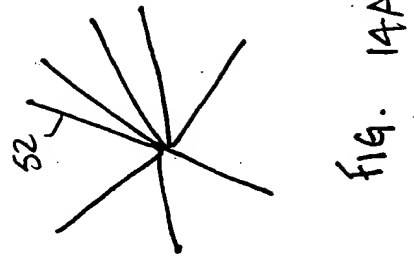
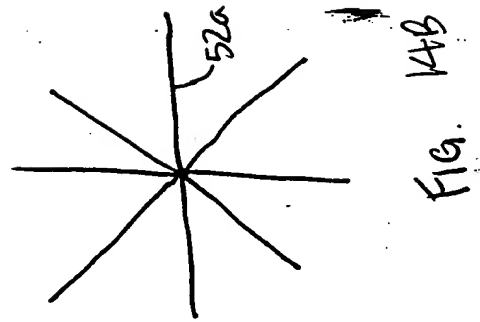
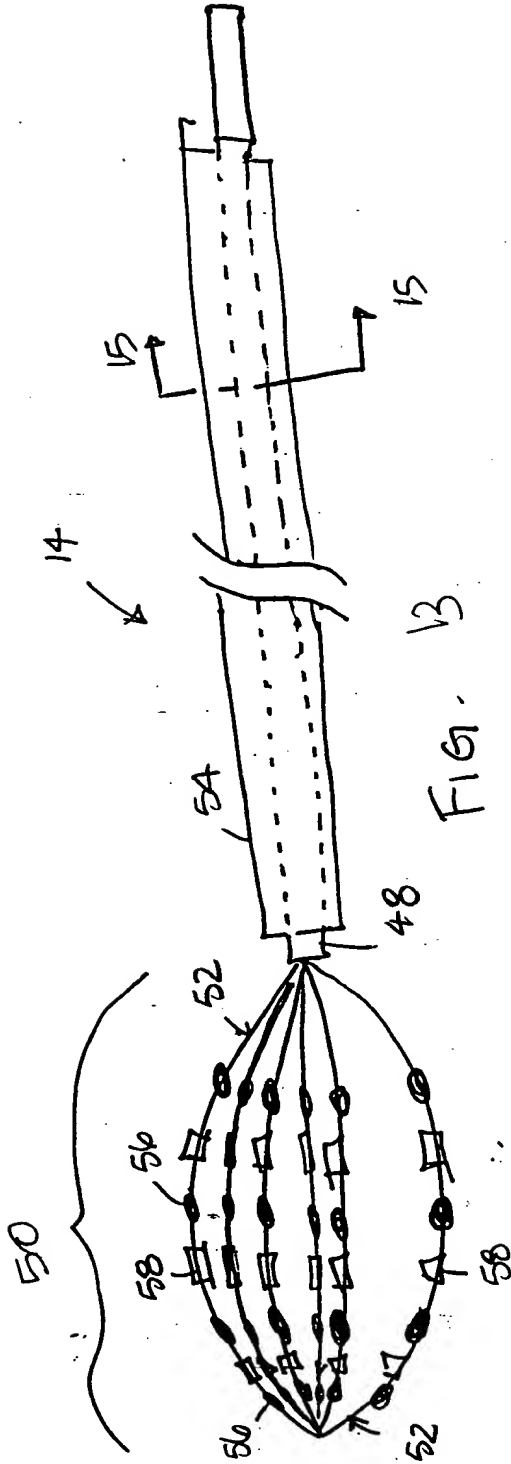


FIGURE 12 DISTAL PLATE TRANSDUCER WITHIN ABLATION CATHETER TIP



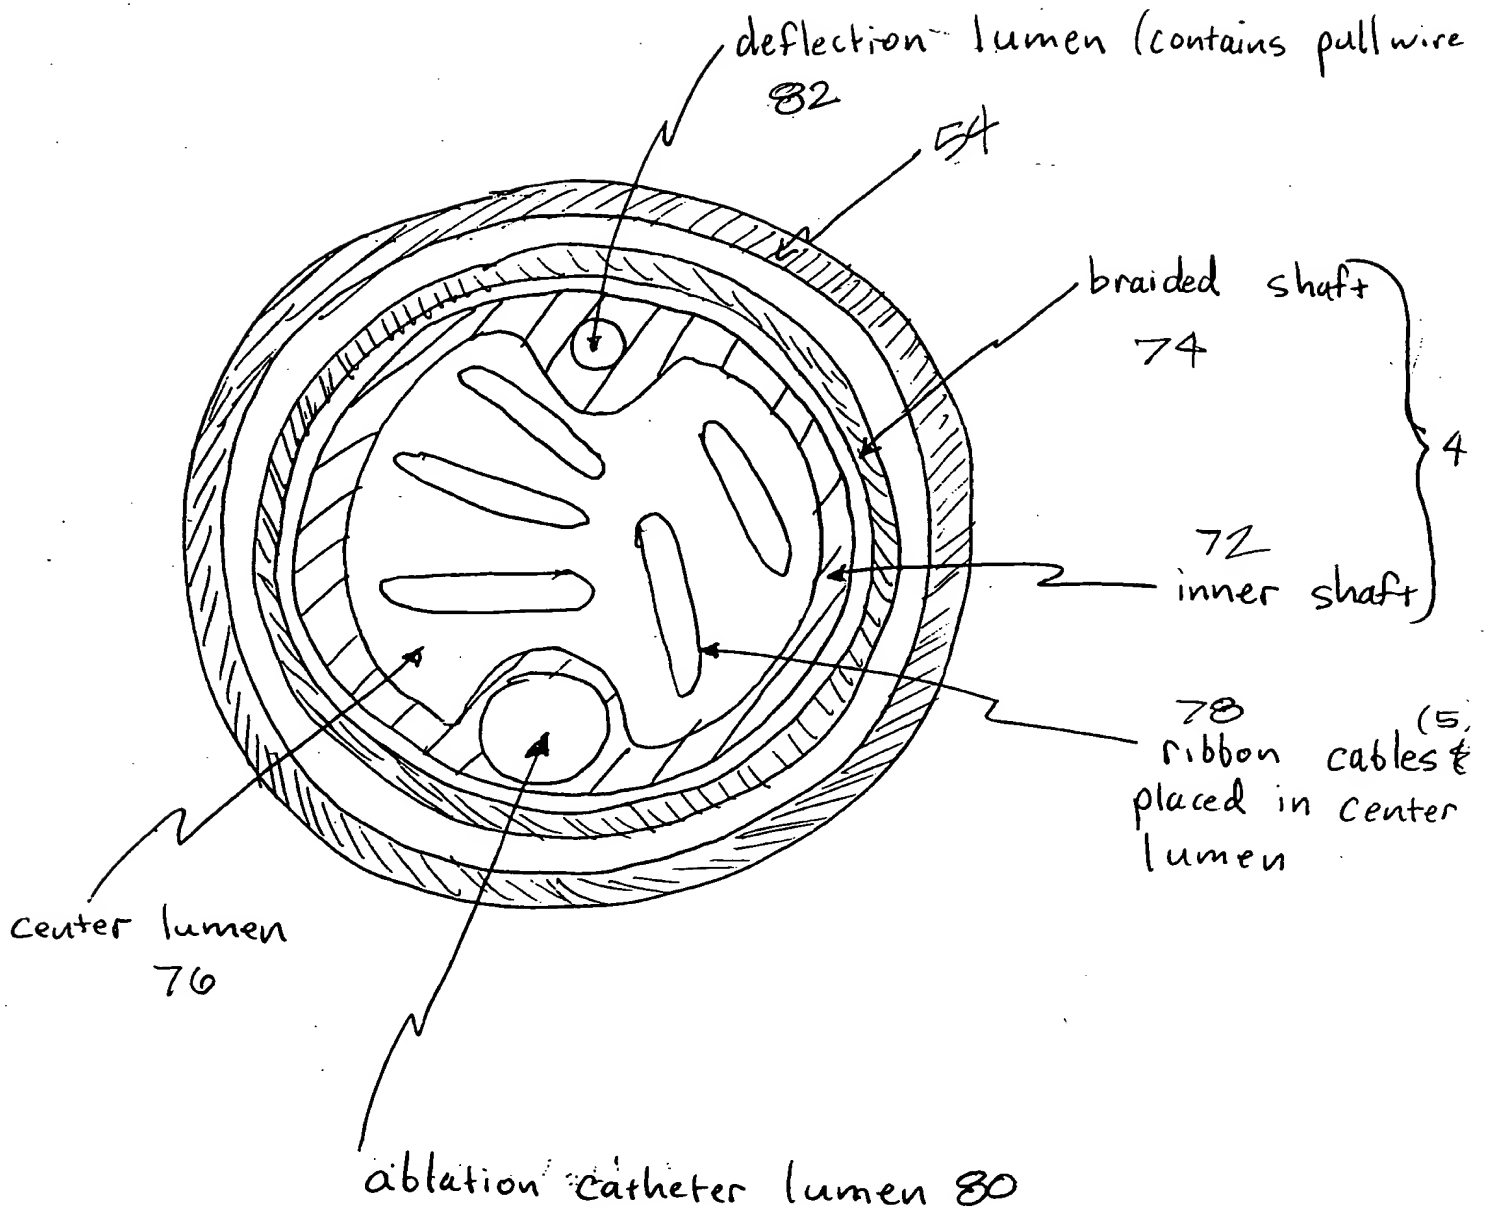
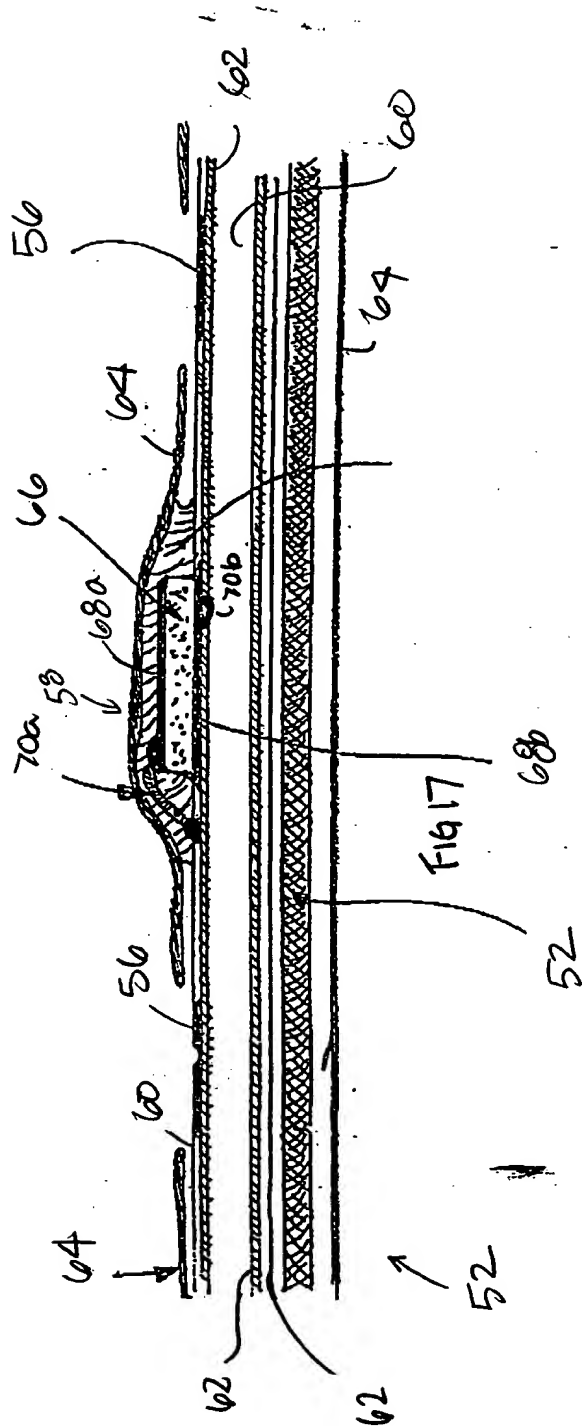
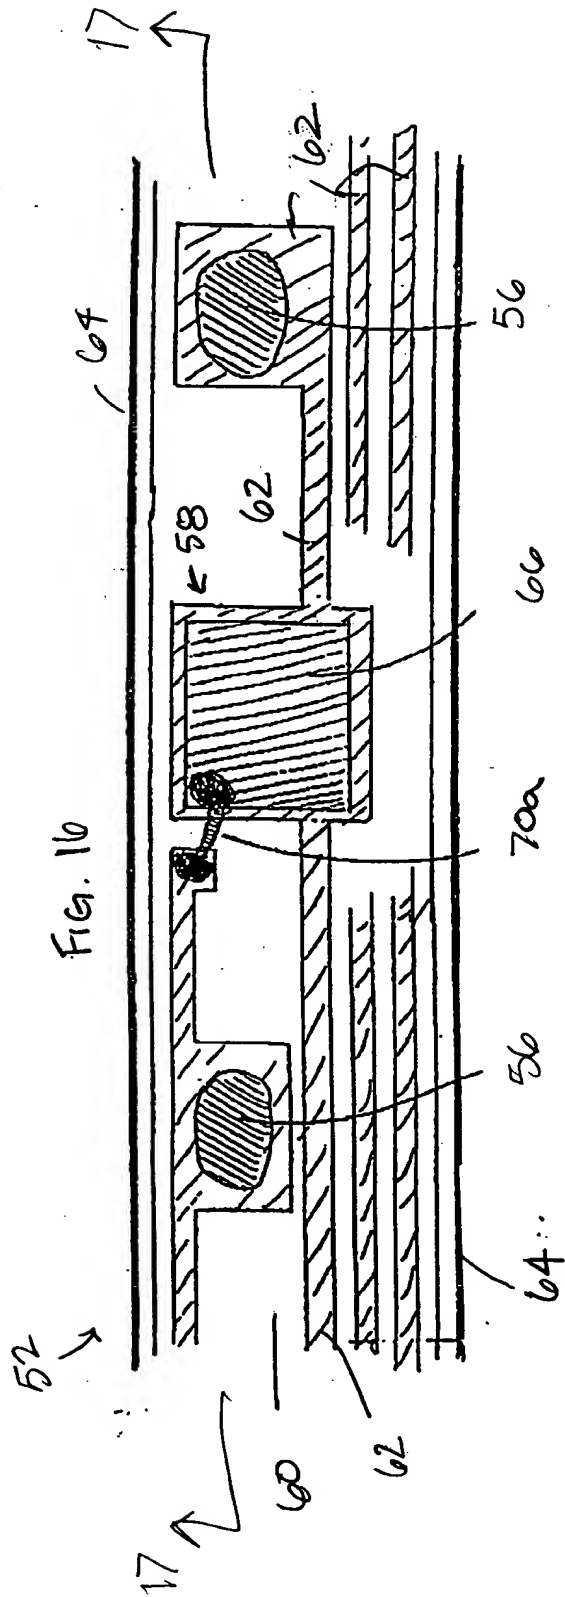


Figure 15 with details



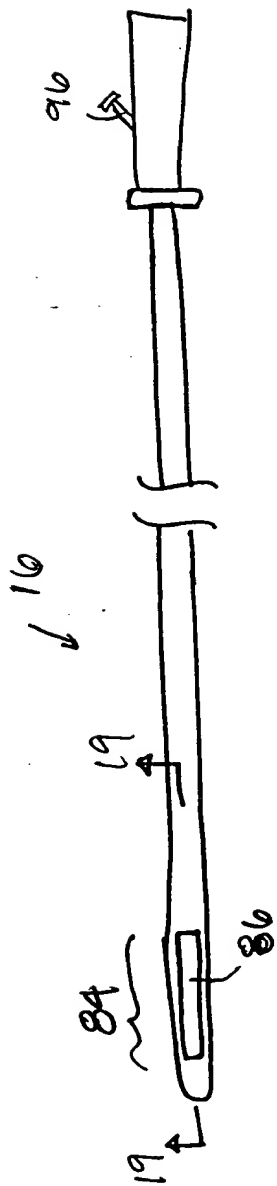


FIG. 18

160



→ 24

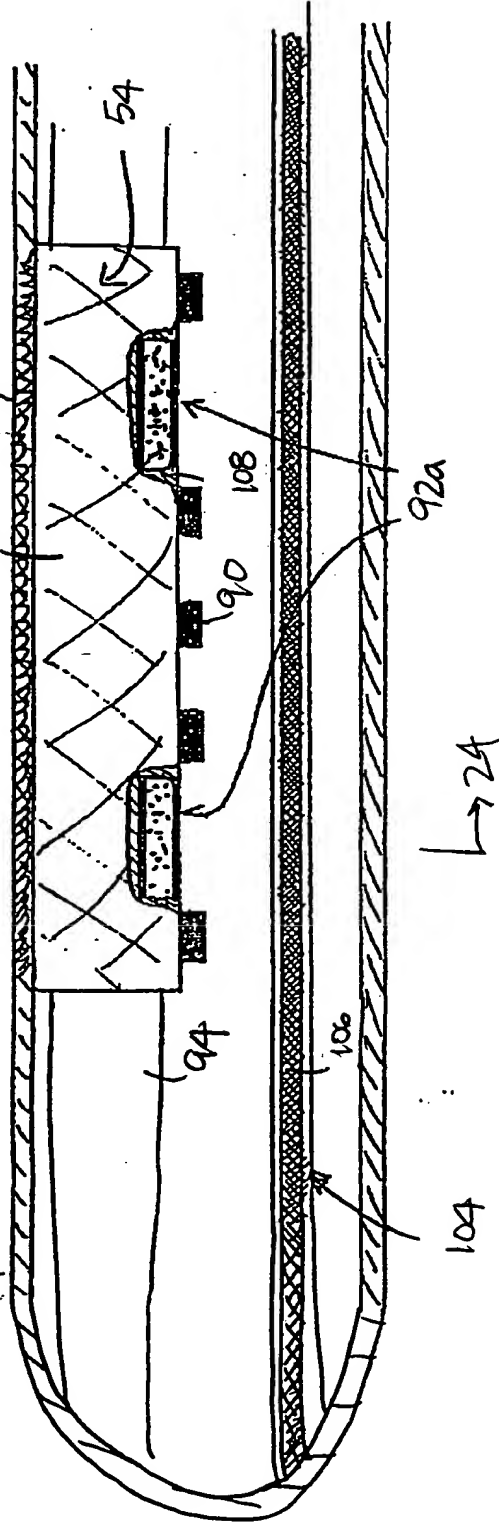


FIG. 23

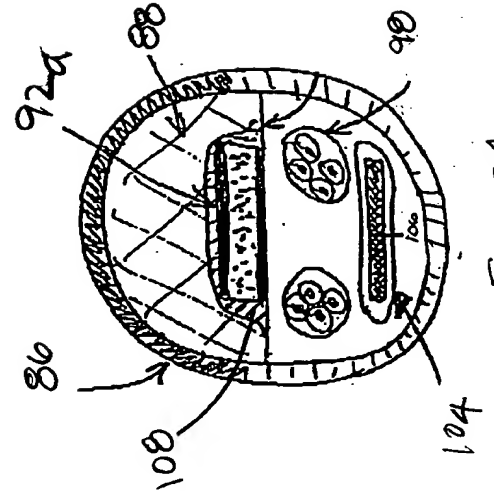


FIG. 24

106

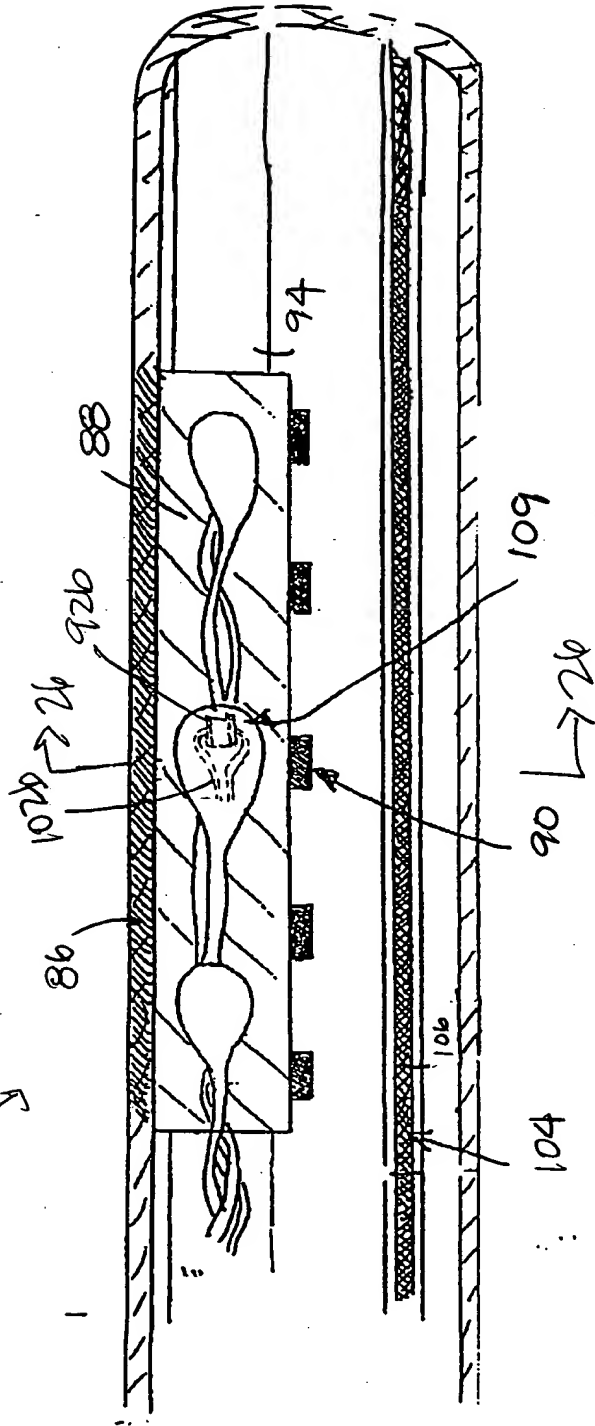


Fig. 25

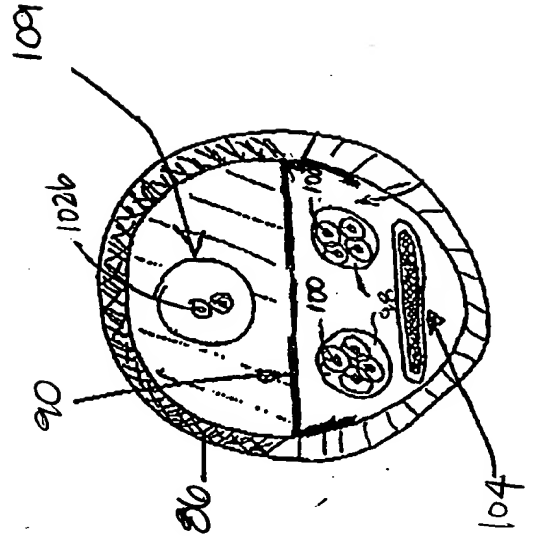
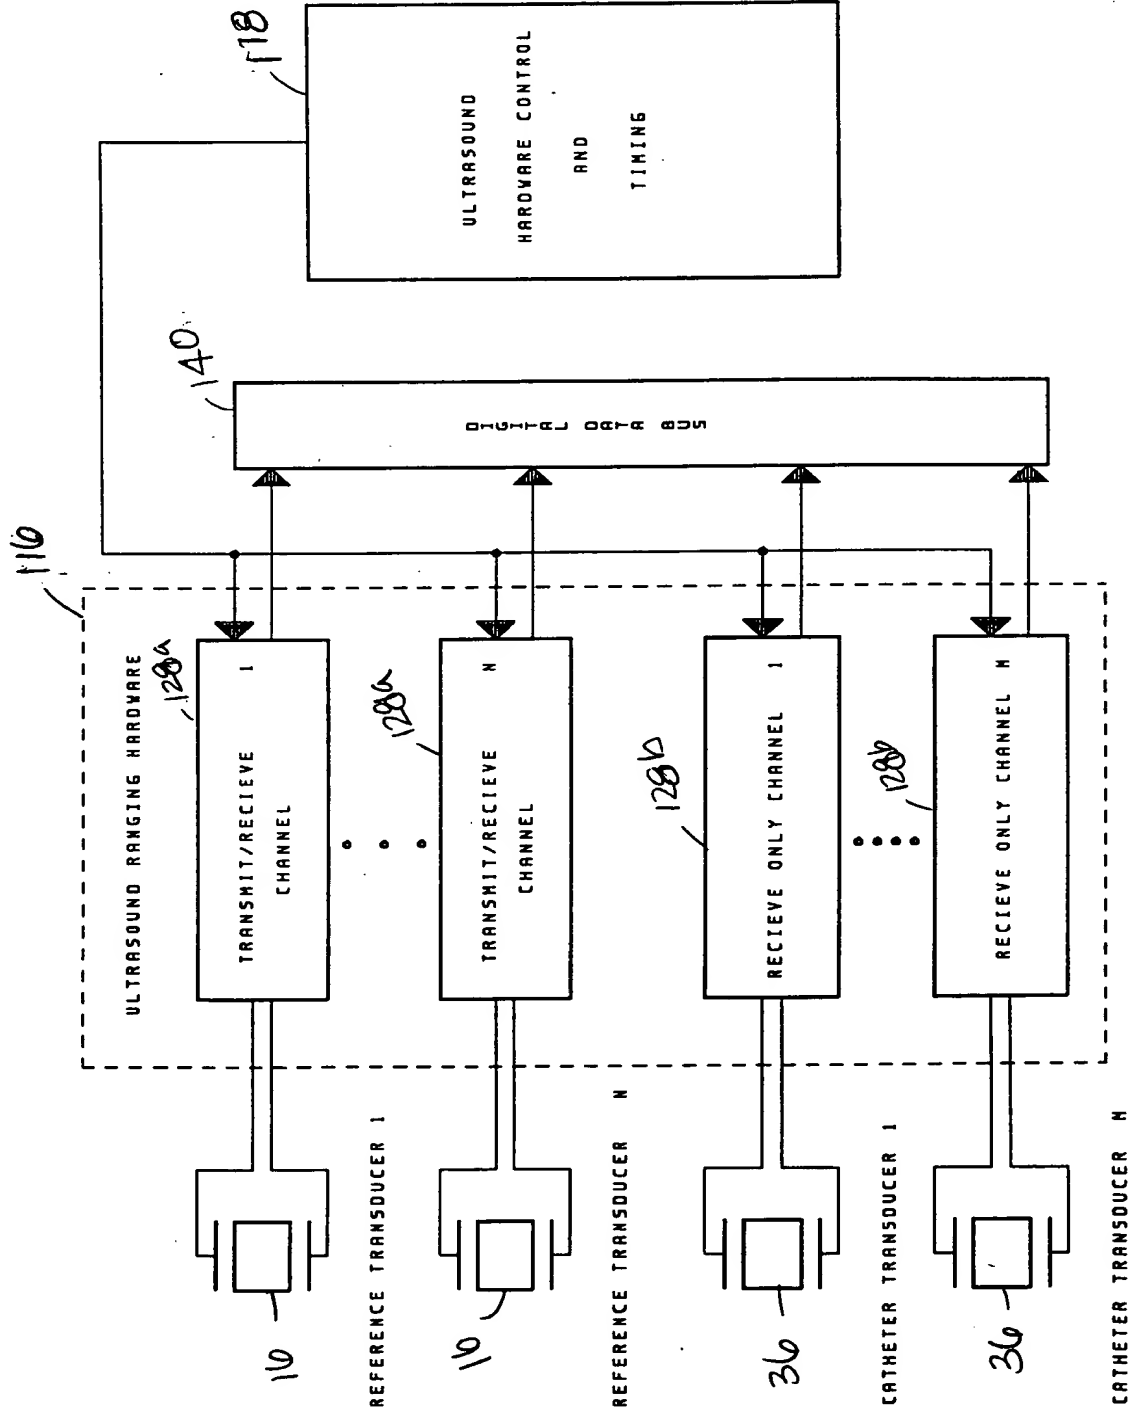
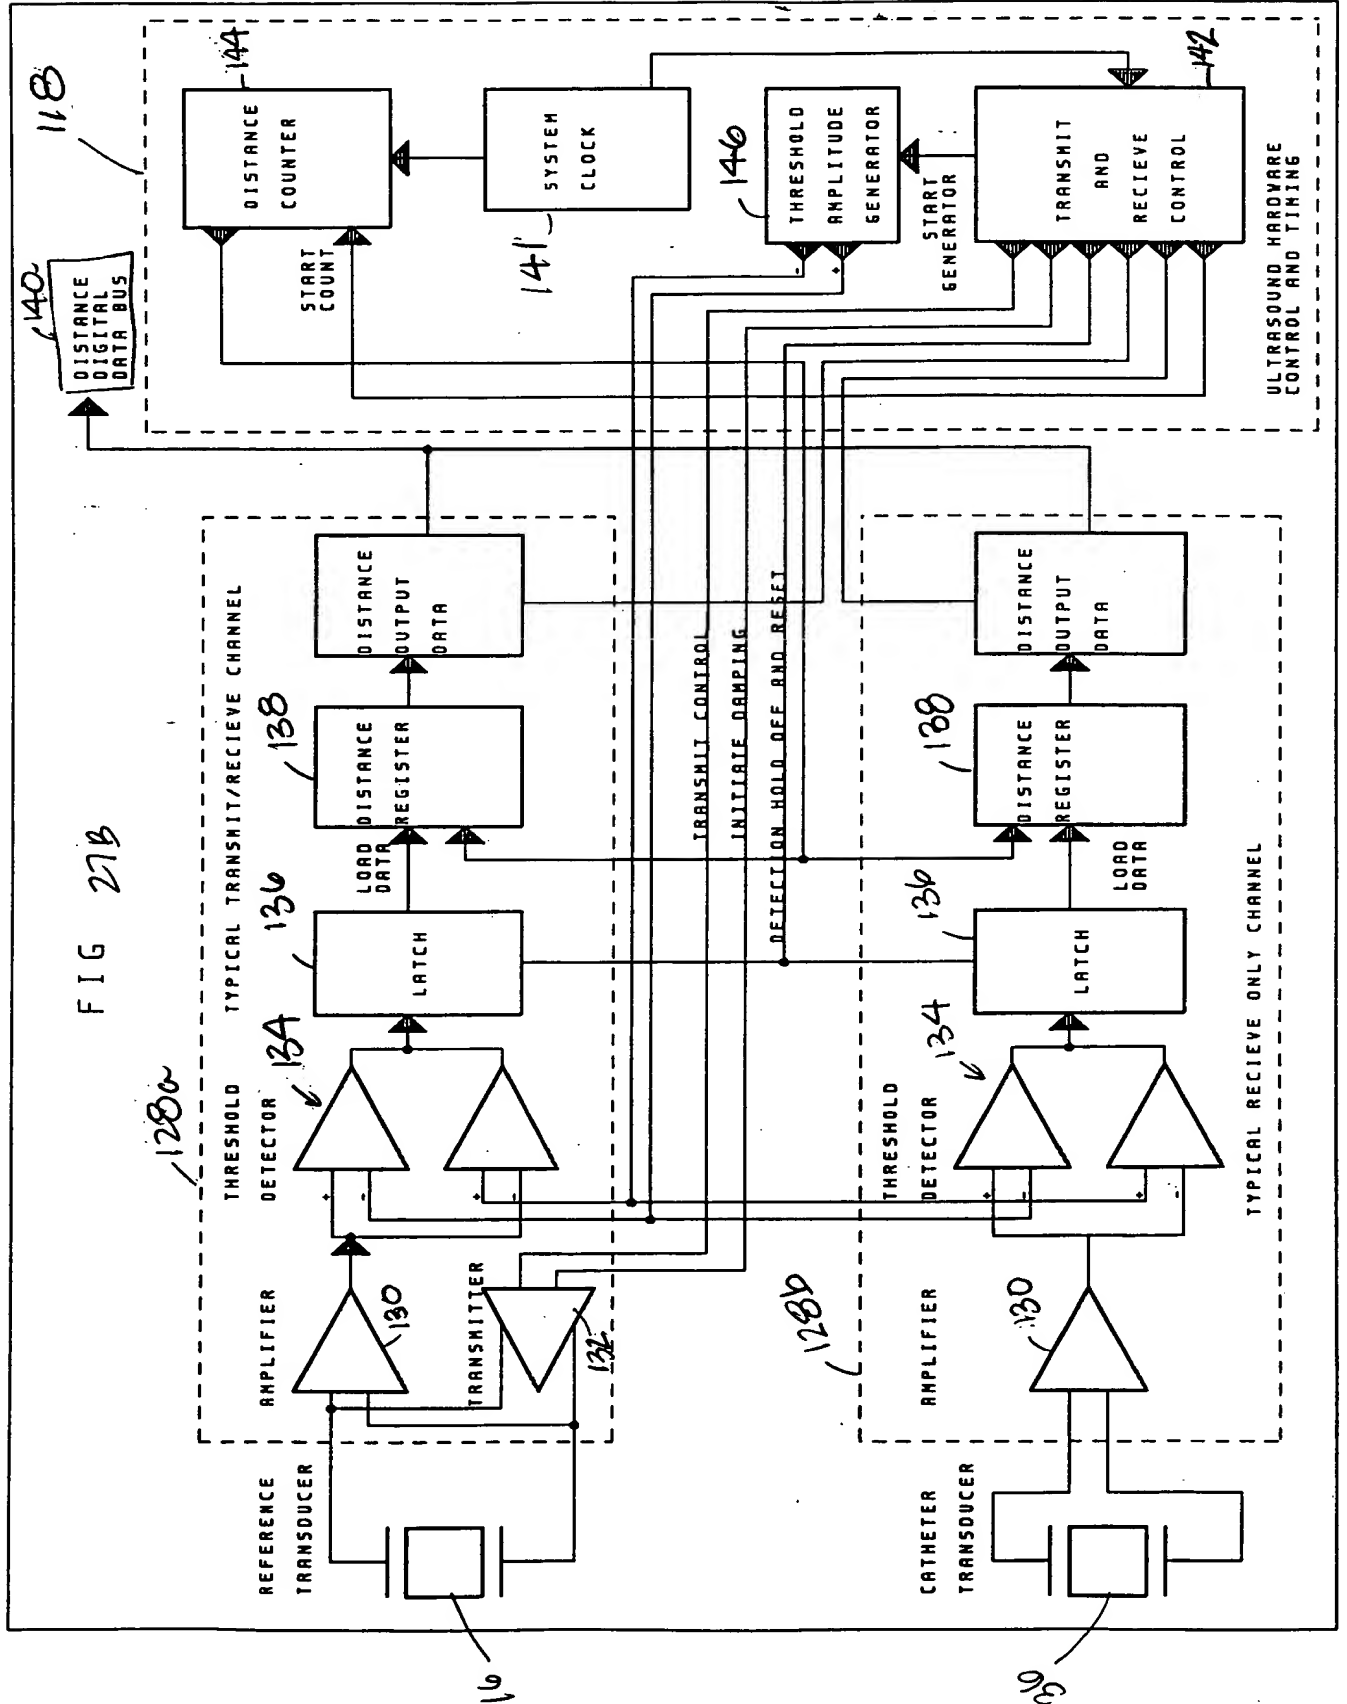


Fig. 26

FIG 27A





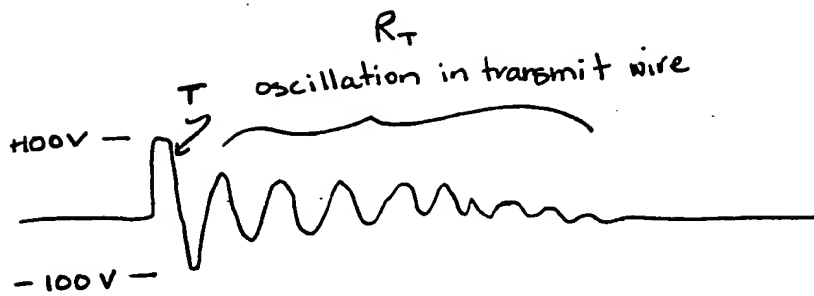


FIG. 28A

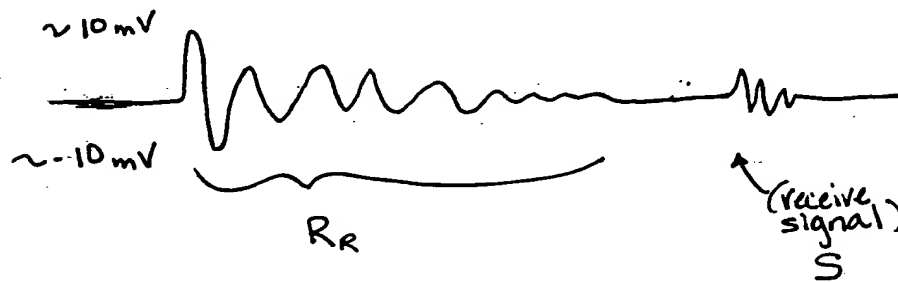


FIG. 28B

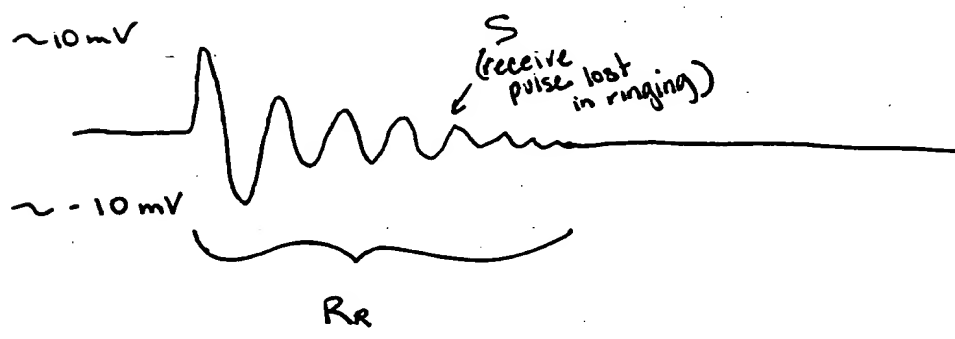


FIG 28C

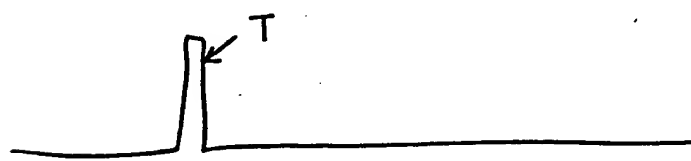


FIG. 28D



FIG 28E

0948304 1080360



Fig. 30A

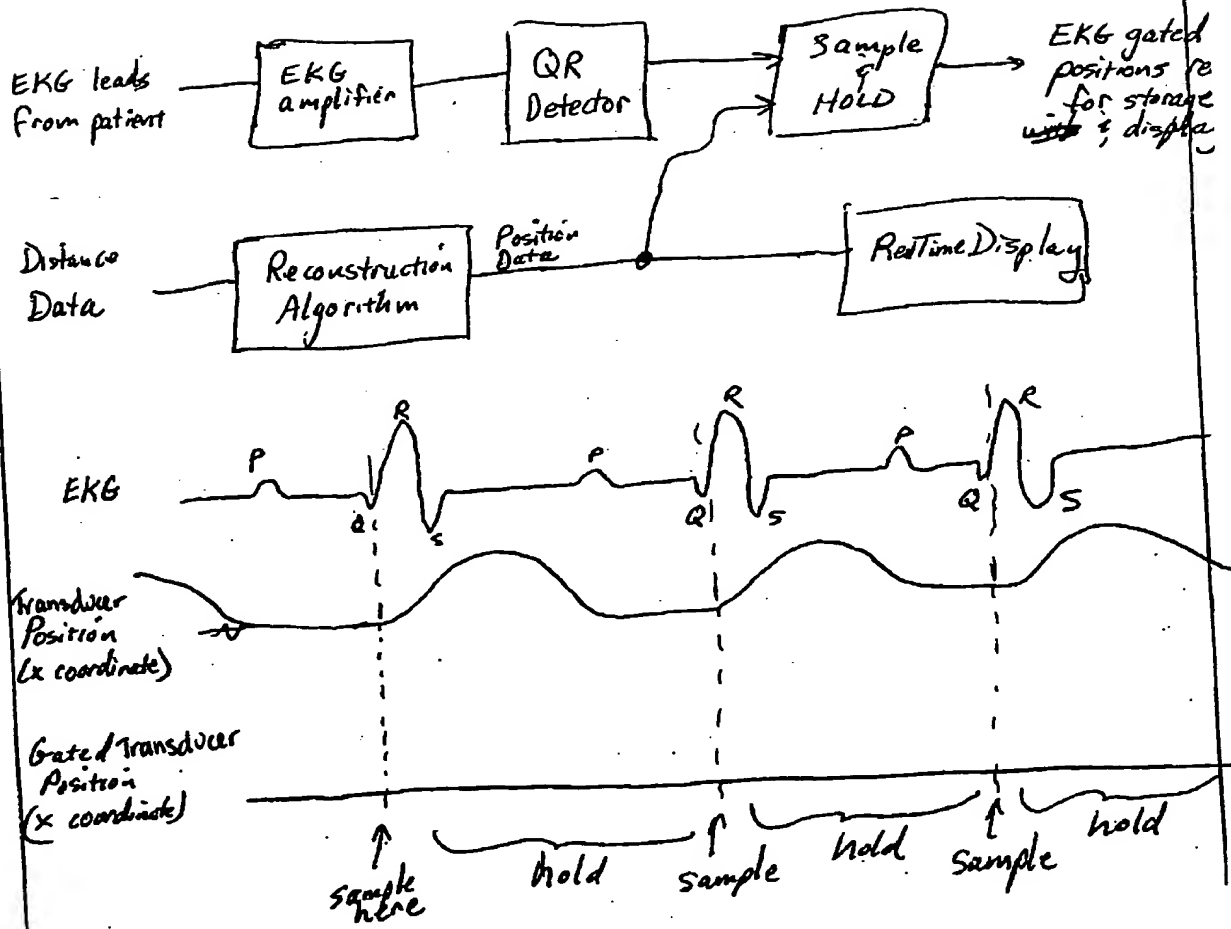


Fig. 30B

3D User Interface

09128304-10822160

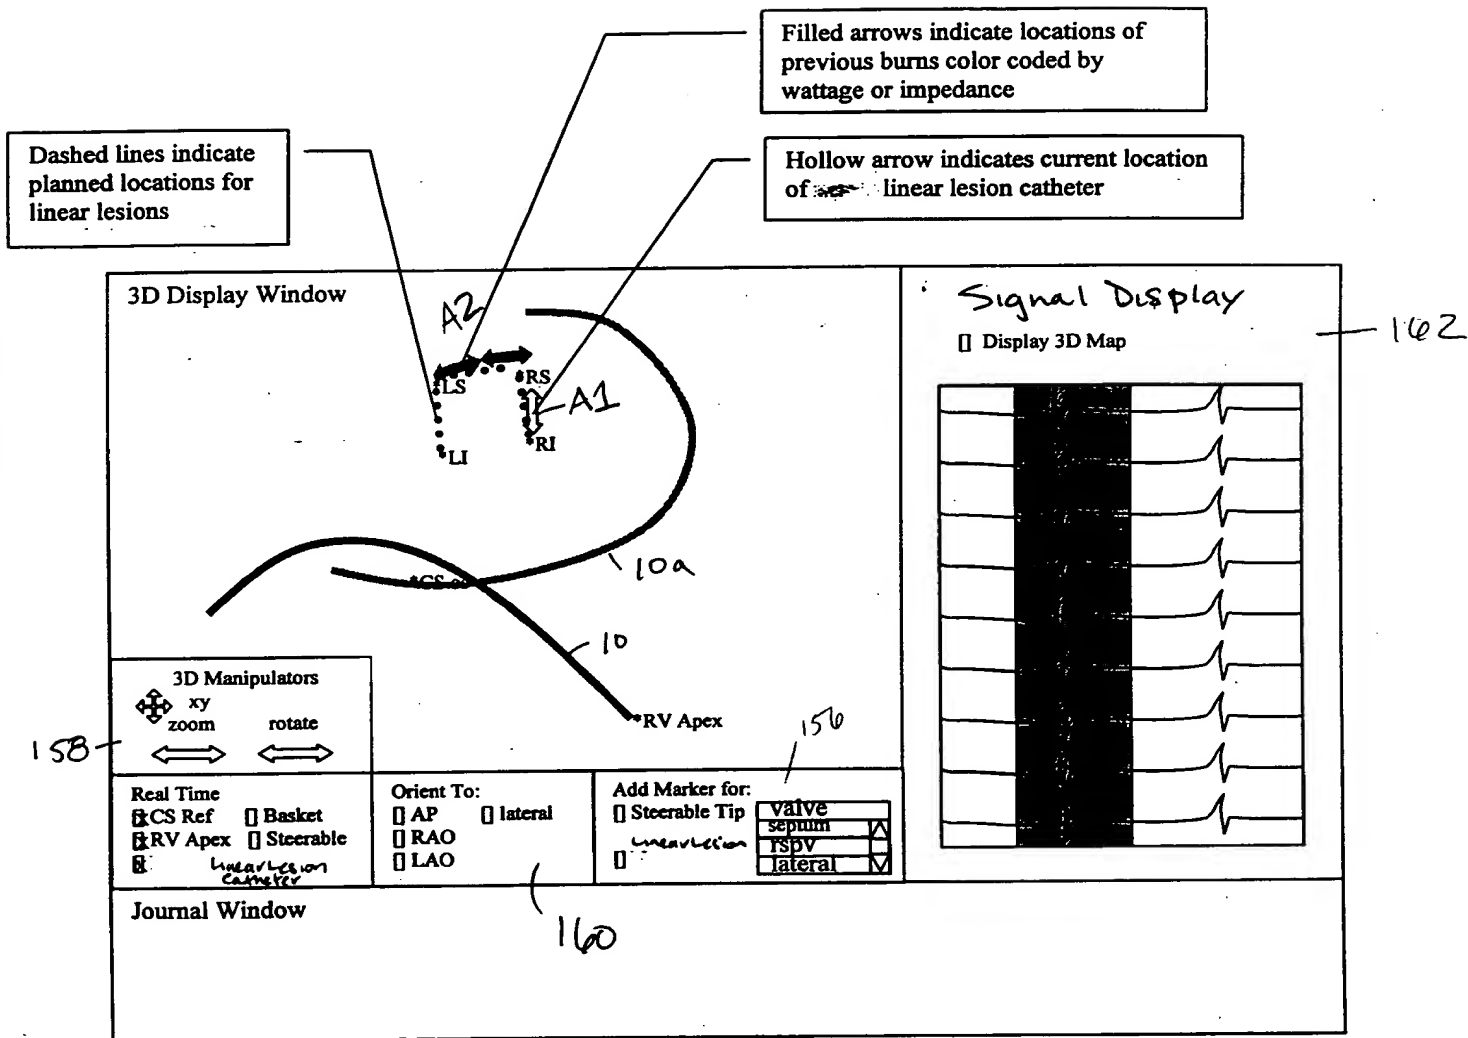


Figure 31

3D Display Window

14, A2, 10a, 10, RV Apex

3D Manipulations

xy zoom rotate

Real Time

ECG Ref ☐ Baseline ☐ Storable ☐ Linearization ☐

RV Apex

156

Journal Window

160


Signal Display

Valve Positions


| | |
|-------|----------|
| Valve | Position |
| 156V | 156V |
| 156V | 156V |

FIG. 32

SECRET



Using the Basket with Integrated Ablation



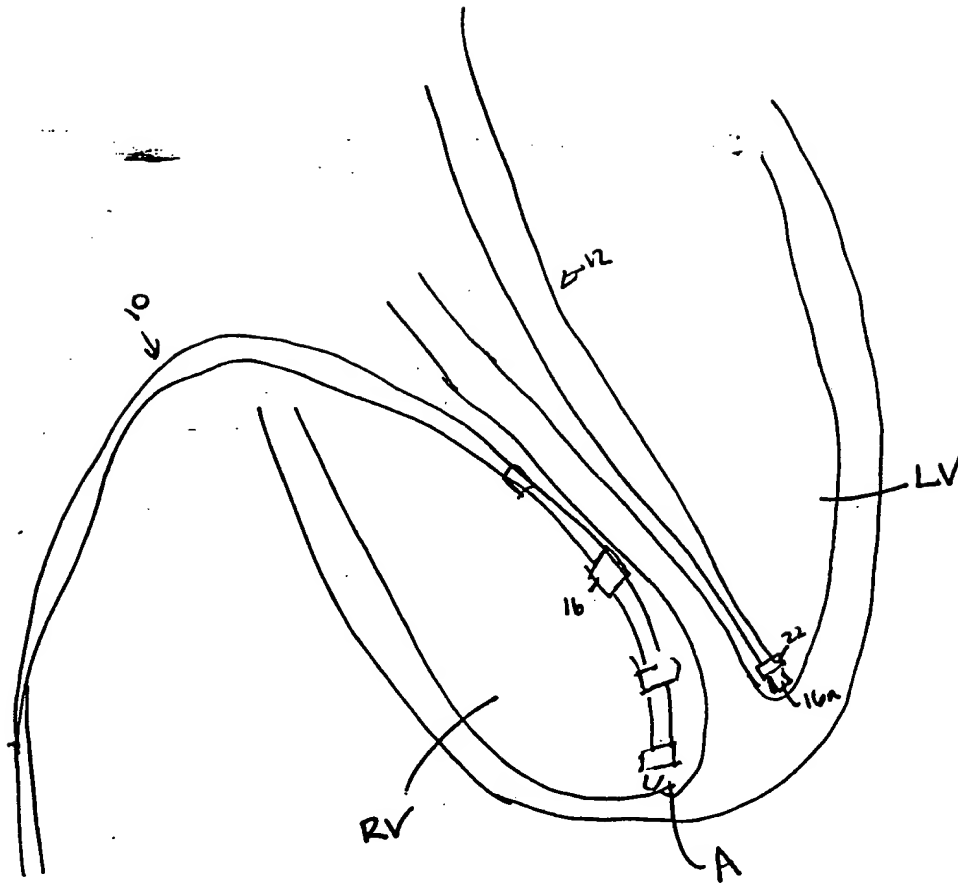


FIG. 3A

0943304.C0000000

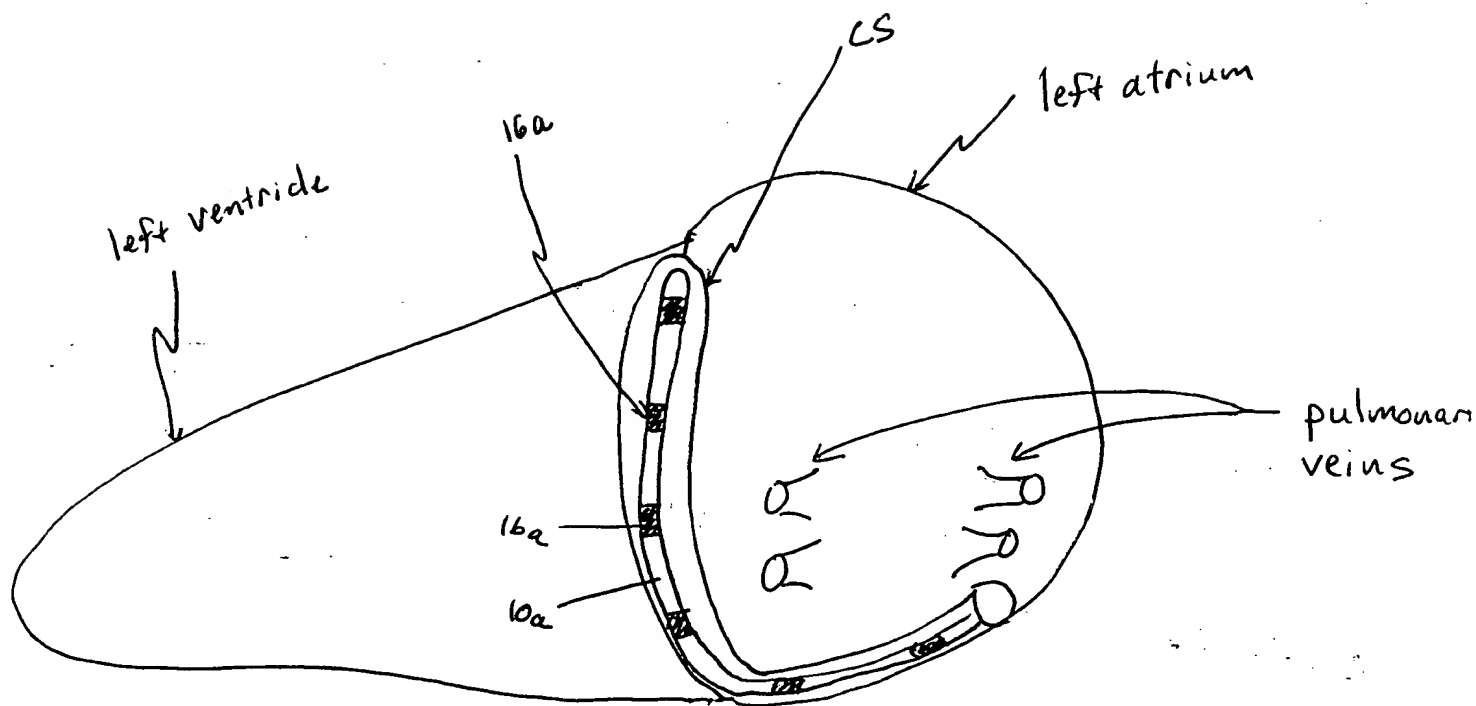


Figure 34B

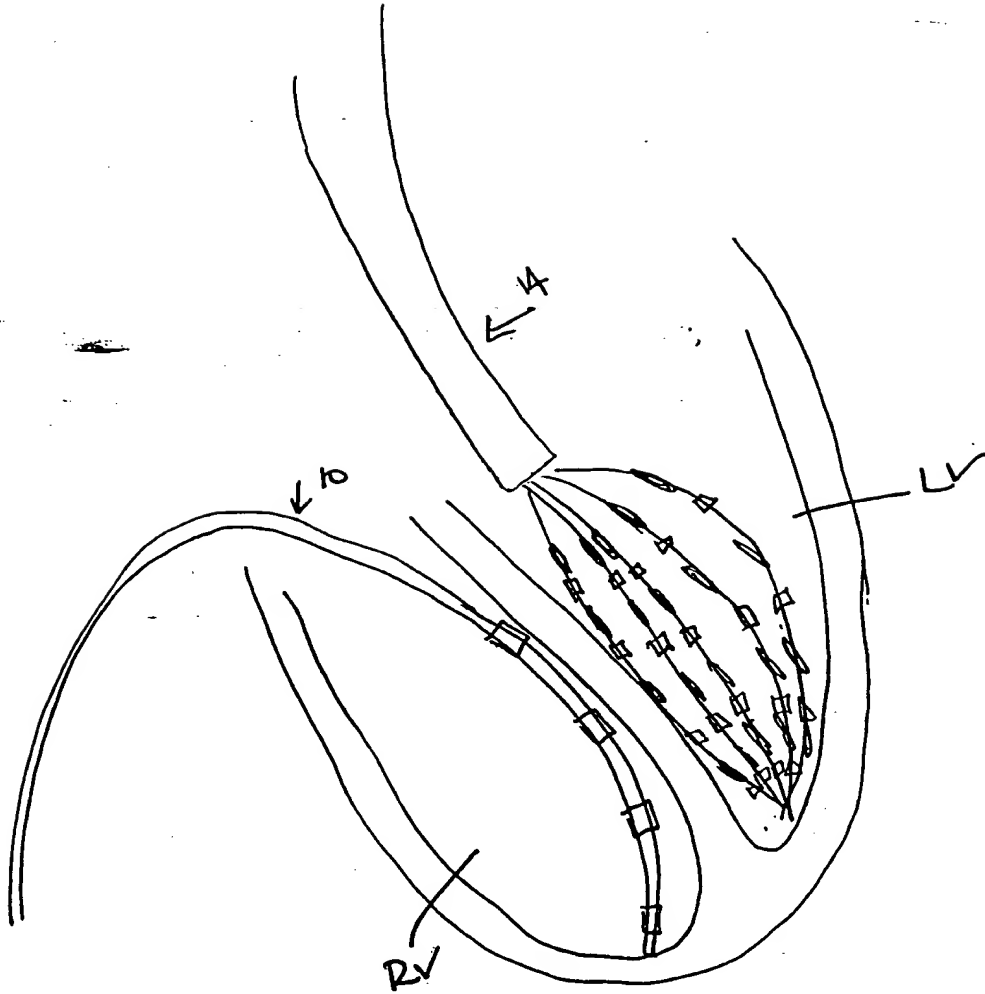


FIG 34C

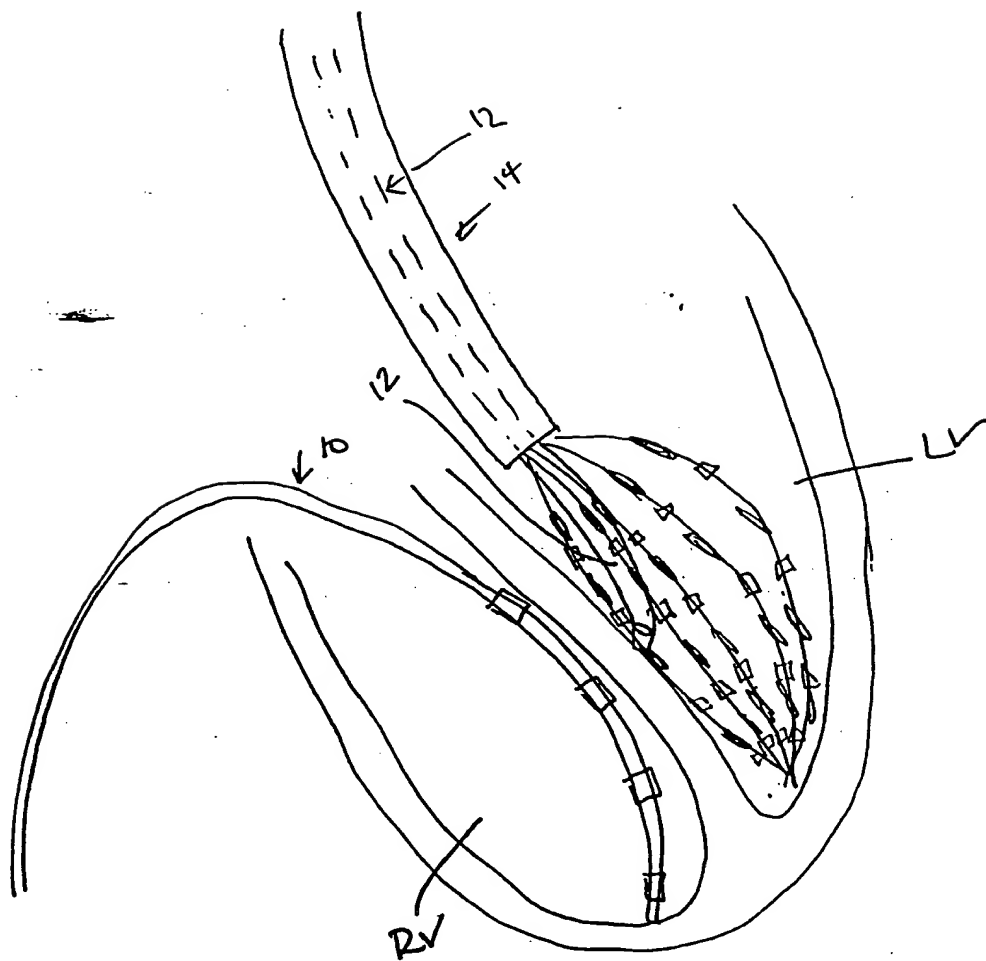


FIG 34B

Clinical Method for Atrial Fibrillation

Device Interaction

Software Interaction

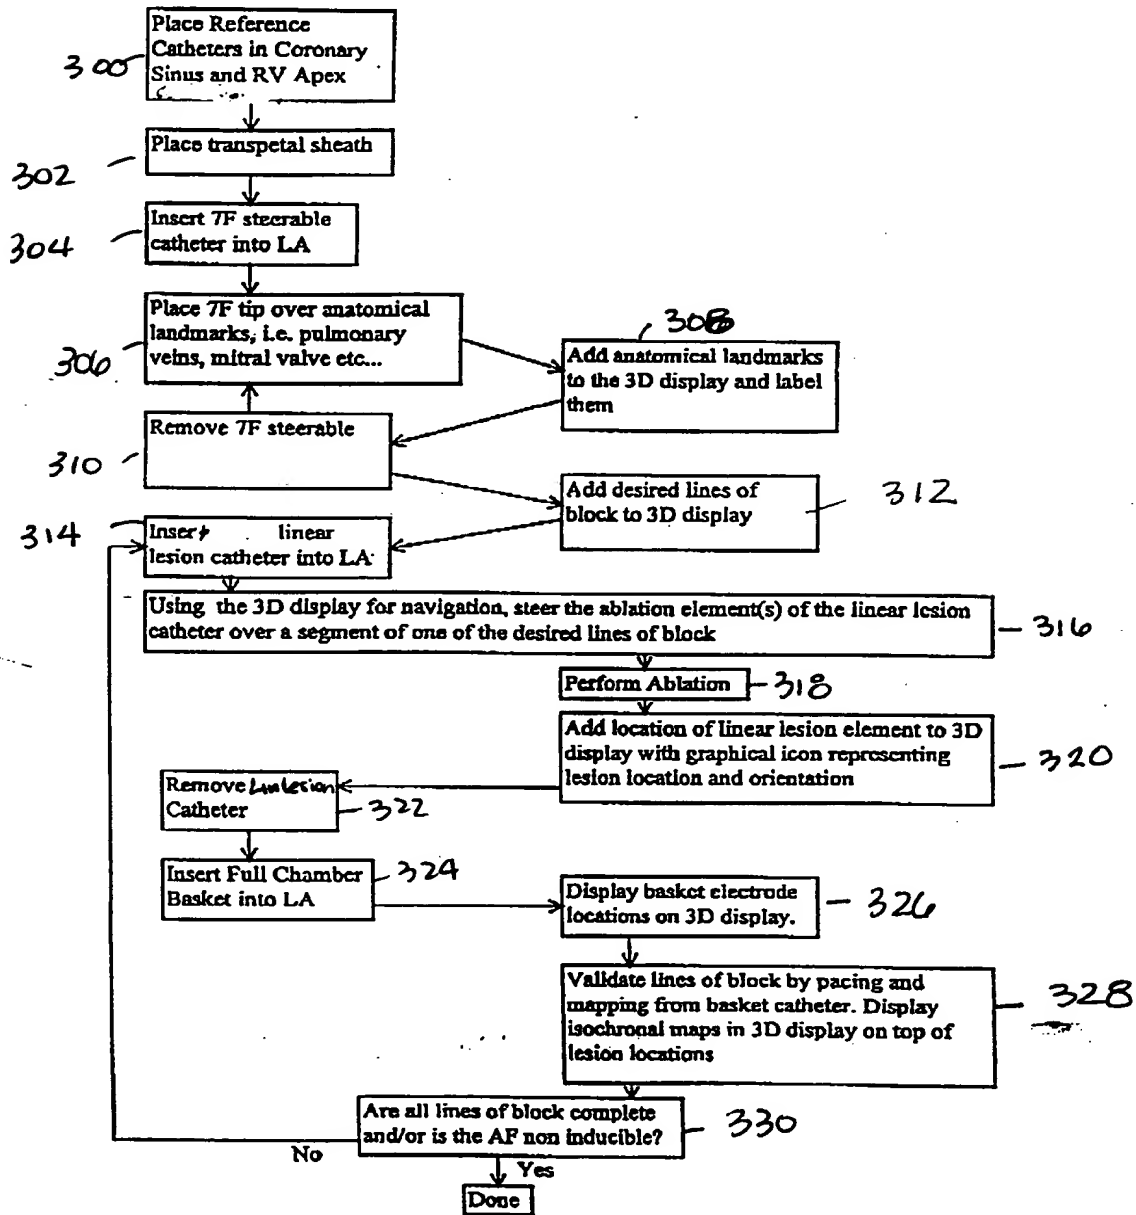


FIG. 35

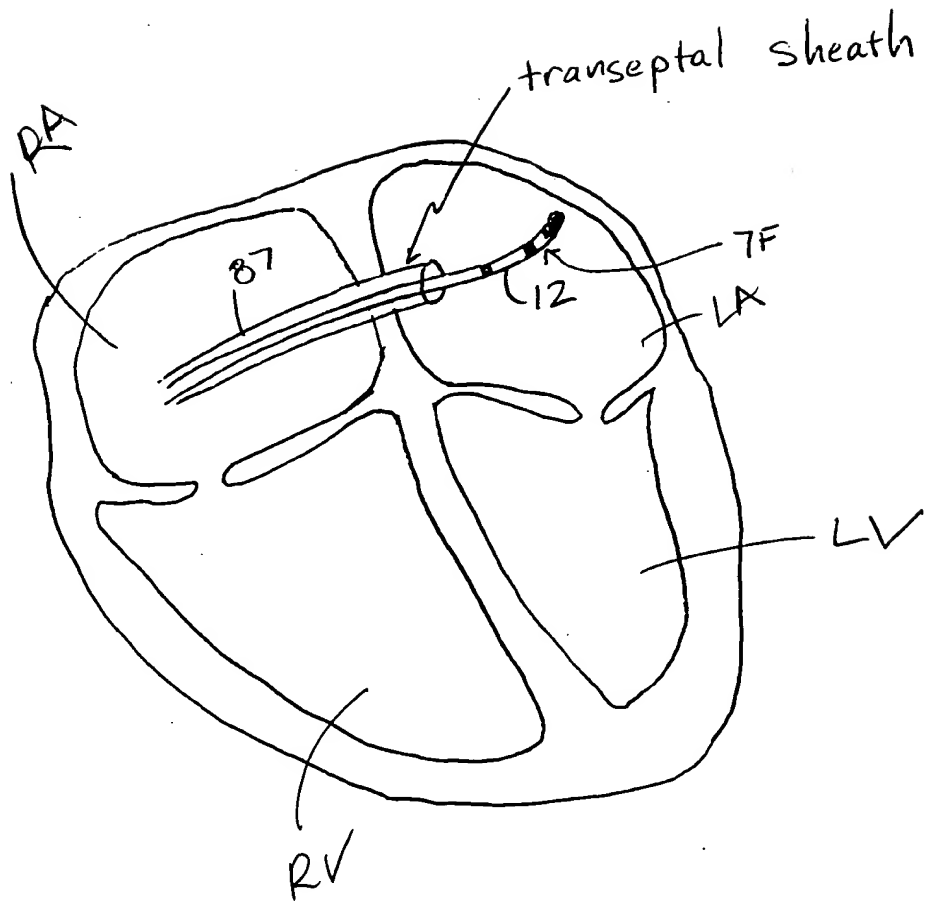


Figure 3bA

09128304.080398
B5E080"40E82T60

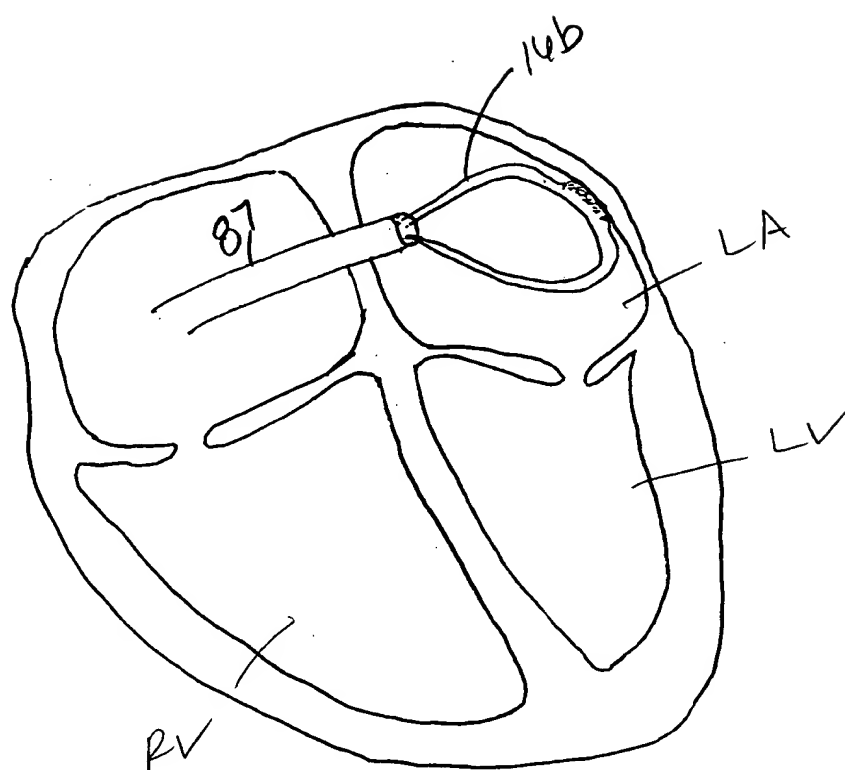


Figure 36b

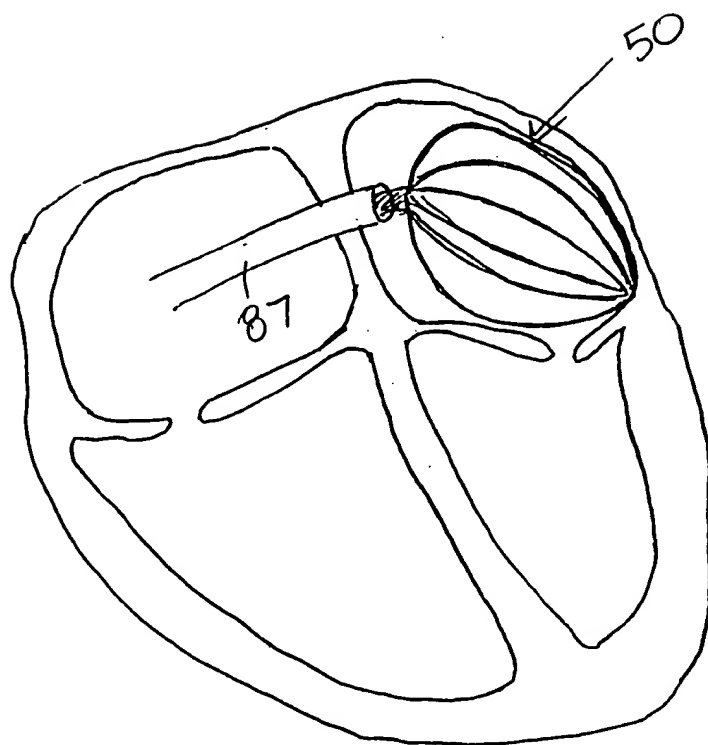


Figure 36C

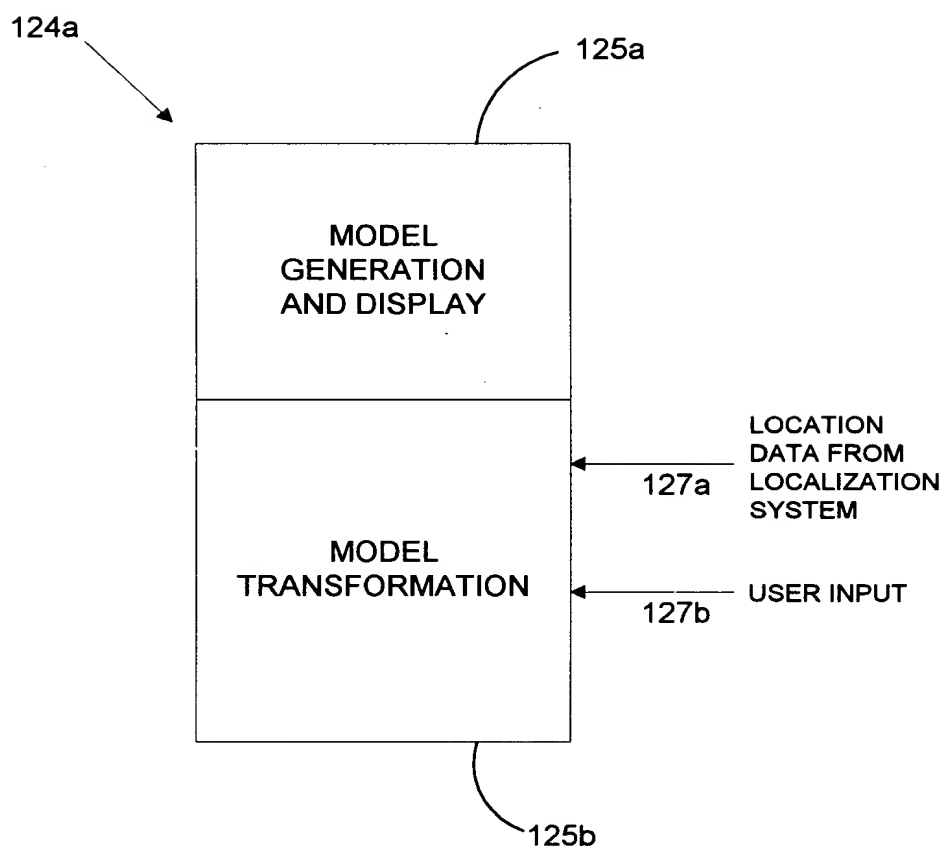


FIG. 37

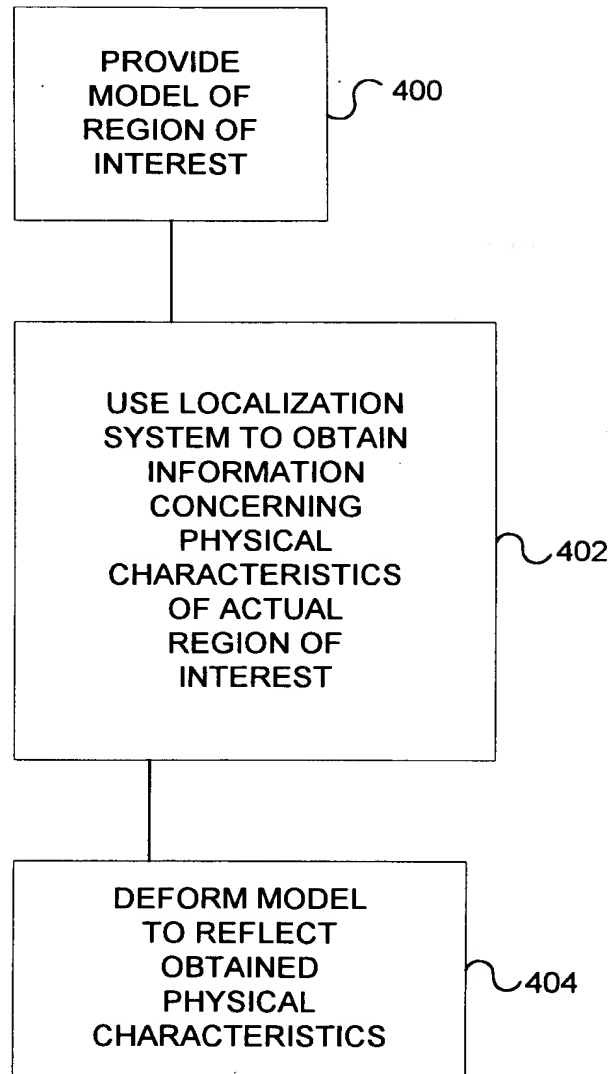
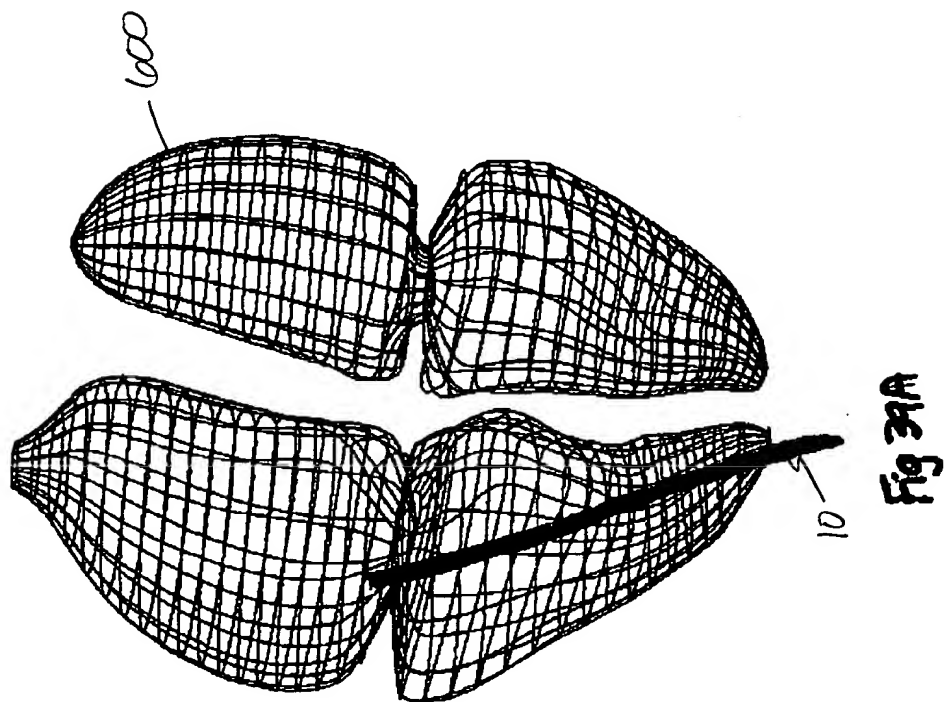
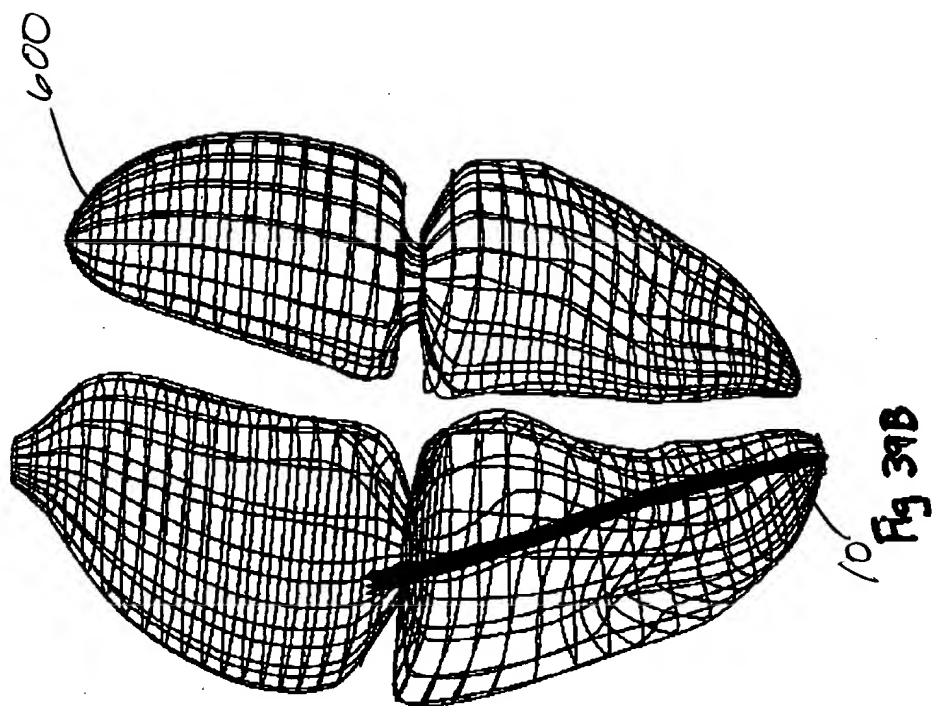


FIG. 38



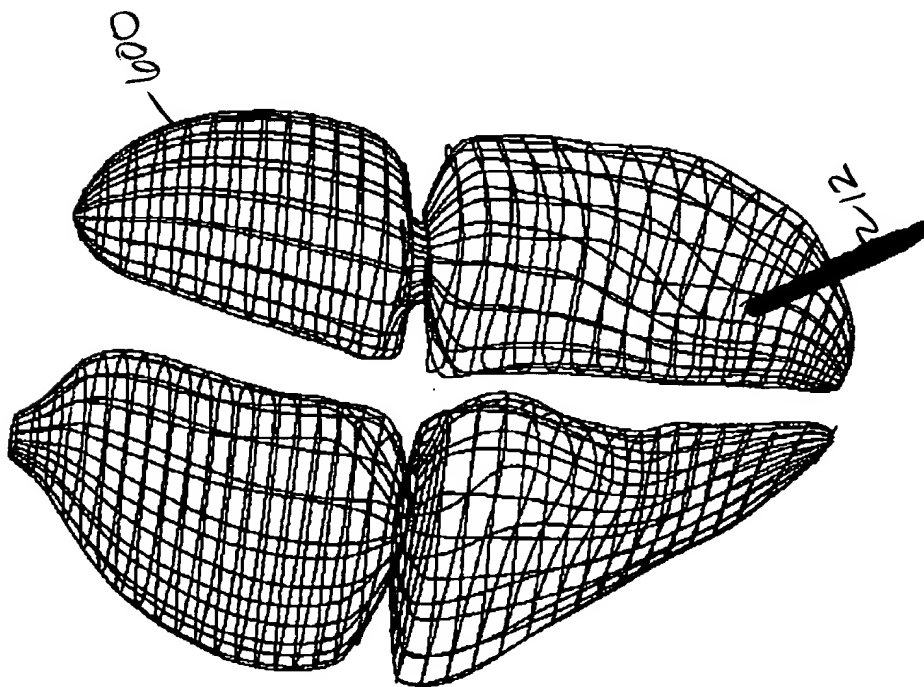


Fig 40A

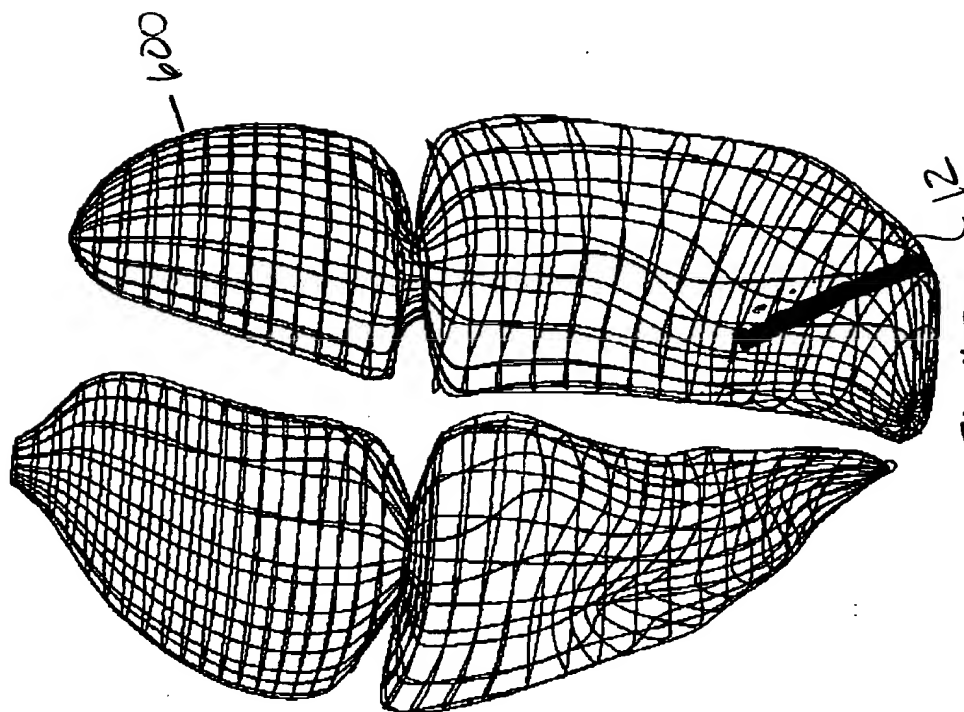


Fig 40B

20250801-102827.60

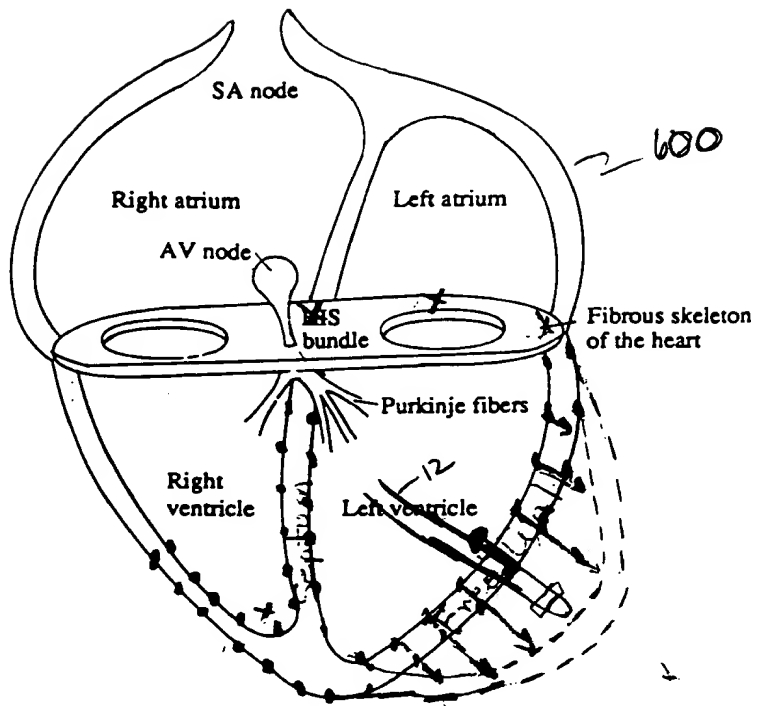


FIG. 400

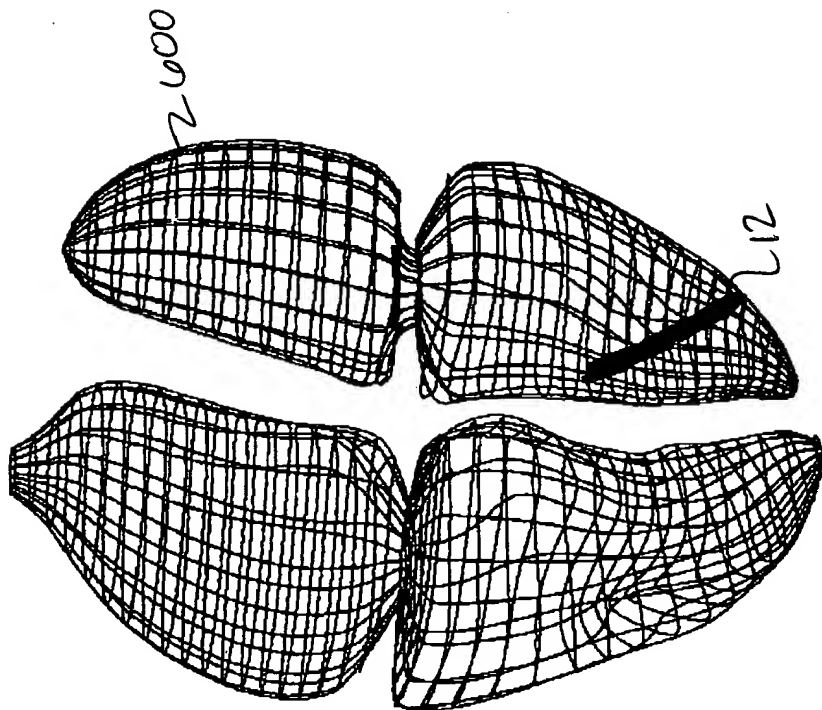


Fig 41B

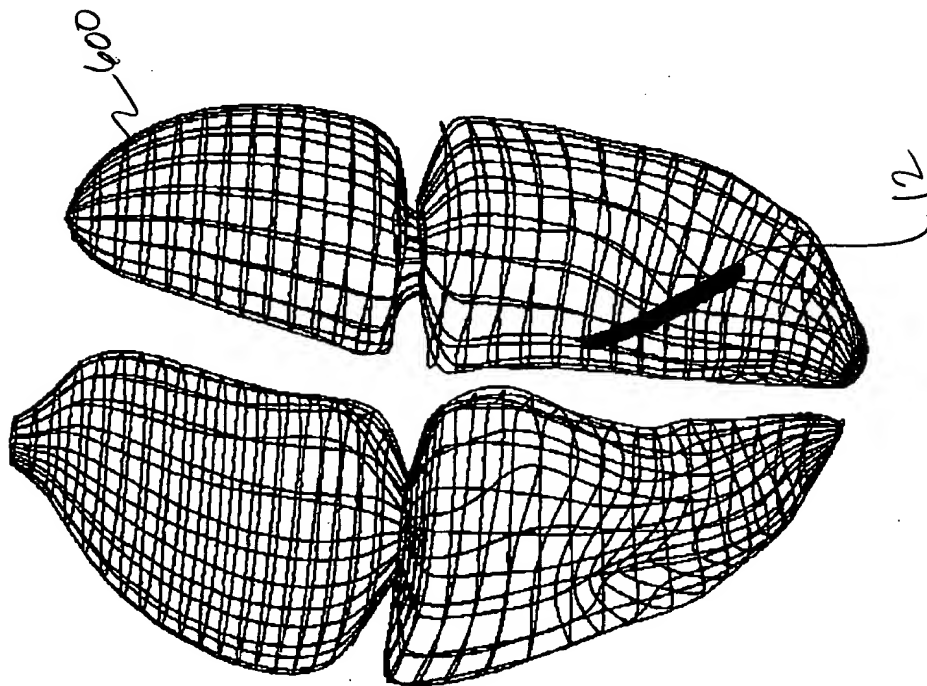


Fig 41A

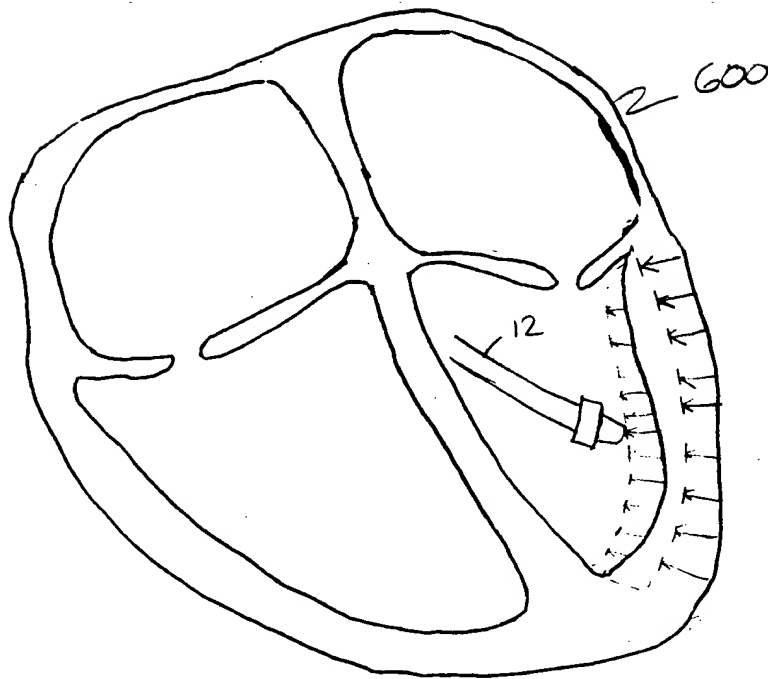


Figure 4C

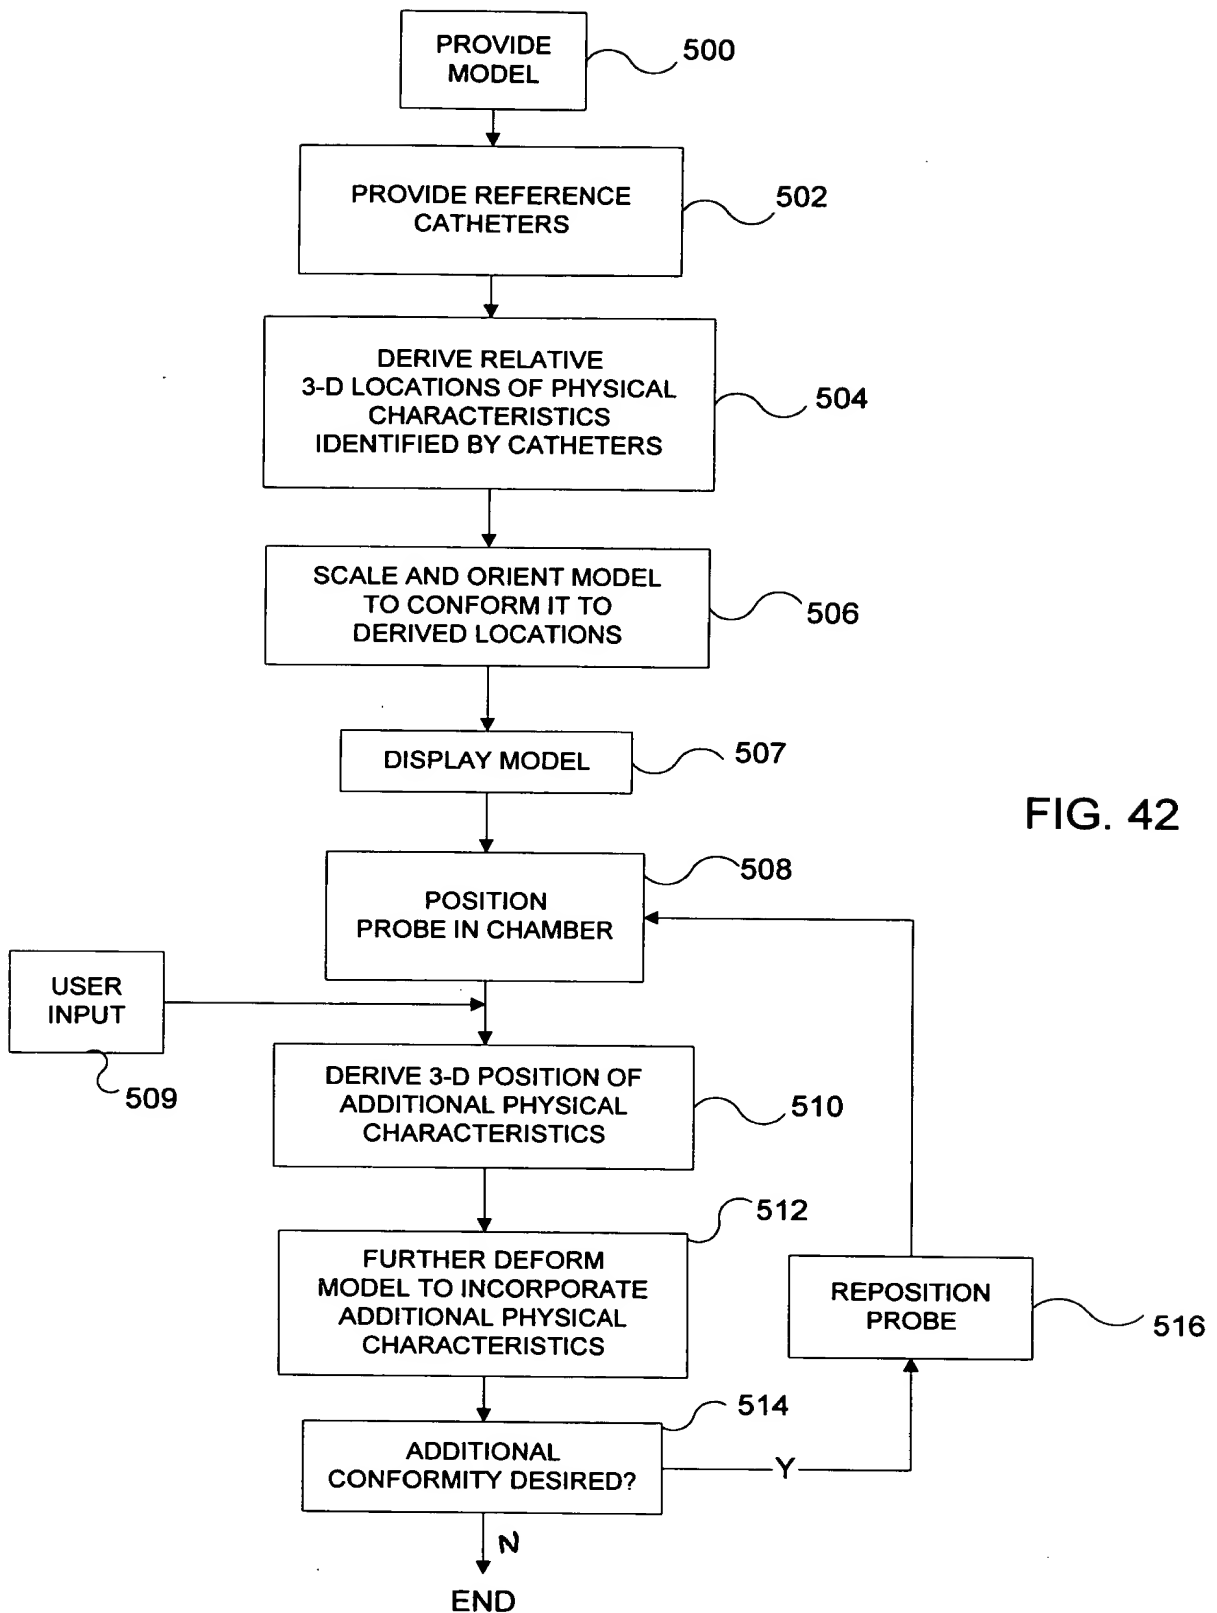


FIG. 42